

ANALYTICAL REPORT

TestAmerica Laboratories, Inc.

TestAmerica Canton
4101 Shuffel Street NW
North Canton, OH 44720
Tel: (330)497-9396

TestAmerica Job ID: 240-108701-1

Client Project/Site: Ford LTP Livonia MI - E203631

For:

ARCADIS U.S., Inc.
28550 Cabot Drive
Suite 500
Novi, Michigan 48377

Attn: Kristoffer Hinskey



Authorized for release by:
3/14/2019 9:59:08 AM

Michael DelMonico, Project Manager I
(330)497-9396
michael.delmonico@testamericainc.com

LINKS

Review your project
results through
TotalAccess

Have a Question?



Visit us at:
www.testamericainc.com

This report has been electronically signed and authorized by the signatory. Electronic signature is intended to be the legally binding equivalent of a traditionally handwritten signature.

Results relate only to the items tested and the sample(s) as received by the laboratory.



Table of Contents

Cover Page	1
Table of Contents	2
Definitions/Glossary	3
Case Narrative	4
Method Summary	5
Sample Summary	6
Detection Summary	7
Client Sample Results	8
Surrogate Summary	99
QC Sample Results	100
QC Association Summary	103
Lab Chronicle	104
Certification Summary	106
Chain of Custody	107

Definitions/Glossary

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Qualifiers

GC/MS VOA

Qualifier	Qualifier Description
U	Indicates the analyte was analyzed for but not detected.
J	Result is less than the RL but greater than or equal to the MDL and the concentration is an approximate value.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Case Narrative

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Job ID: 240-108701-1

Laboratory: TestAmerica Canton

Narrative

CASE NARRATIVE

Client: ARCADIS U.S., Inc.

Project: Ford LTP Livonia MI - E203631

Report Number: 240-108701-1

With the exceptions noted as flags or footnotes, standard analytical protocols were followed in the analysis of the samples and no problems were encountered or anomalies observed. In addition all laboratory quality control samples were within established control limits, with any exceptions noted below. Each sample was analyzed to achieve the lowest possible reporting limit within the constraints of the method. In some cases, due to interference or analytes present at high concentrations, samples were diluted. For diluted samples, the reporting limits are adjusted relative to the dilution required.

TestAmerica Canton attests to the validity of the laboratory data generated by TestAmerica facilities reported herein. All analyses performed by TestAmerica facilities were done using established laboratory SOPs that incorporate QA/QC procedures described in the application methods. TestAmerica's operations groups have reviewed the data for compliance with the laboratory QA/QC plan, and data have been found to be compliant with laboratory protocols unless otherwise noted below.

The test results in this report meet all NELAP requirements for parameters for which accreditation is required or available. Any exceptions to NELAP requirements are noted in this report. Pursuant to NELAP, this report may not be reproduced, except in full, without the written approval of the laboratory.

Calculations are performed before rounding to avoid round-off errors in calculated results.

All holding times were met and proper preservation noted for the methods performed on these samples, unless otherwise detailed in the individual sections below.

All solid sample results are reported on an "as received" basis unless otherwise indicated by the presence of a % solids value in the method header.

This laboratory report is confidential and is intended for the sole use of TestAmerica and its client.

RECEIPT

The samples were received on 2/28/2019 8:00 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 2.6° C.

VOLATILE ORGANIC COMPOUNDS (GCMS)

Samples MW-131S_022619 (240-108701-1), MW-132S_022619 (240-108701-2), MW-85_022619 (240-108701-3), MW-78S_022619 (240-108701-4), MW-78_022619 (240-108701-5) and TRIP BLANK (240-108701-6) were analyzed for volatile organic compounds (GCMS) in accordance with EPA SW-846 Method 8260B. The samples were analyzed on 03/01/2019.

No analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

VOLATILE ORGANIC COMPOUNDS (GCMS SIM)

Samples MW-131S_022619 (240-108701-1), MW-132S_022619 (240-108701-2), MW-85_022619 (240-108701-3), MW-78S_022619 (240-108701-4) and MW-78_022619 (240-108701-5) were analyzed for volatile organic compounds (GCMS SIM) in accordance with EPA SW-846 Method 8260B SIM. The samples were analyzed on 03/02/2019.

No analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Method Summary

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Method	Method Description	Protocol	Laboratory
8260B	Volatile Organic Compounds (GC/MS)	SW846	TAL CAN
8260B SIM	Volatile Organic Compounds (GC/MS)	SW846	TAL CAN
5030B	Purge and Trap	SW846	TAL CAN

Protocol References:

SW846 = "Test Methods For Evaluating Solid Waste, Physical/Chemical Methods", Third Edition, November 1986 And Its Updates.

Laboratory References:

TAL CAN = TestAmerica Canton, 4101 Shuffel Street NW, North Canton, OH 44720, TEL (330)497-9396

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

Sample Summary

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
240-108701-1	MW-131S_022619	Water	02/26/19 09:47	02/28/19 08:00
240-108701-2	MW-132S_022619	Water	02/26/19 11:22	02/28/19 08:00
240-108701-3	MW-85_022619	Water	02/26/19 13:23	02/28/19 08:00
240-108701-4	MW-78S_022619	Water	02/26/19 15:47	02/28/19 08:00
240-108701-5	MW-78_022619	Water	02/26/19 16:40	02/28/19 08:00
240-108701-6	TRIP BLANK	Water	02/26/19 00:00	02/28/19 08:00

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

Detection Summary

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-131S_022619

Lab Sample ID: 240-108701-1

Analyte	Result	Qualifier	RL	MDL	Unit	Dil Fac	D	Method	Prep Type
Vinyl chloride	0.69	J	1.0	0.20	ug/L	1		8260B	Total/NA

Client Sample ID: MW-132S_022619

Lab Sample ID: 240-108701-2

No Detections.

Client Sample ID: MW-85_022619

Lab Sample ID: 240-108701-3

Analyte	Result	Qualifier	RL	MDL	Unit	Dil Fac	D	Method	Prep Type
Vinyl chloride	5.5		1.0	0.20	ug/L	1		8260B	Total/NA

Client Sample ID: MW-78S_022619

Lab Sample ID: 240-108701-4

No Detections.

Client Sample ID: MW-78_022619

Lab Sample ID: 240-108701-5

Analyte	Result	Qualifier	RL	MDL	Unit	Dil Fac	D	Method	Prep Type
cis-1,2-Dichloroethene	0.22	J	1.0	0.16	ug/L	1		8260B	Total/NA

Client Sample ID: TRIP BLANK

Lab Sample ID: 240-108701-6

No Detections.

This Detection Summary does not include radiochemical test results.

TestAmerica Canton

Client Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-131S_022619

Lab Sample ID: 240-108701-1

Date Collected: 02/26/19 09:47

Matrix: Water

Date Received: 02/28/19 08:00

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,4-Dioxane	2.0	U	2.0	0.86	ug/L			03/02/19 18:58	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	85		63 - 125					03/02/19 18:58	1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 19:47	1
cis-1,2-Dichloroethene	1.0	U	1.0	0.16	ug/L			03/01/19 19:47	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 19:47	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 19:47	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 19:47	1
Vinyl chloride	0.69	J	1.0	0.20	ug/L			03/01/19 19:47	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	93		70 - 121					03/01/19 19:47	1
4-Bromofluorobenzene (Surr)	67		59 - 120					03/01/19 19:47	1
Toluene-d8 (Surr)	74		70 - 123					03/01/19 19:47	1
Dibromofluoromethane (Surr)	94		75 - 128					03/01/19 19:47	1

Client Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-132S_022619

Lab Sample ID: 240-108701-2

Date Collected: 02/26/19 11:22

Matrix: Water

Date Received: 02/28/19 08:00

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,4-Dioxane	2.0	U	2.0	0.86	ug/L			03/02/19 19:23	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	82		63 - 125					03/02/19 19:23	1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 20:09	1
cis-1,2-Dichloroethene	1.0	U	1.0	0.16	ug/L			03/01/19 20:09	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 20:09	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 20:09	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 20:09	1
Vinyl chloride	1.0	U	1.0	0.20	ug/L			03/01/19 20:09	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	98		70 - 121					03/01/19 20:09	1
4-Bromofluorobenzene (Surr)	69		59 - 120					03/01/19 20:09	1
Toluene-d8 (Surr)	76		70 - 123					03/01/19 20:09	1
Dibromofluoromethane (Surr)	102		75 - 128					03/01/19 20:09	1

Client Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-85_022619

Lab Sample ID: 240-108701-3

Date Collected: 02/26/19 13:23

Matrix: Water

Date Received: 02/28/19 08:00

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,4-Dioxane	2.0	U	2.0	0.86	ug/L			03/02/19 19:48	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	81		63 - 125					03/02/19 19:48	1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 20:31	1
cis-1,2-Dichloroethene	1.0	U	1.0	0.16	ug/L			03/01/19 20:31	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 20:31	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 20:31	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 20:31	1
Vinyl chloride	5.5		1.0	0.20	ug/L			03/01/19 20:31	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	93		70 - 121					03/01/19 20:31	1
4-Bromofluorobenzene (Surr)	65		59 - 120					03/01/19 20:31	1
Toluene-d8 (Surr)	72		70 - 123					03/01/19 20:31	1
Dibromofluoromethane (Surr)	91		75 - 128					03/01/19 20:31	1

Client Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-78S_022619

Lab Sample ID: 240-108701-4

Date Collected: 02/26/19 15:47

Matrix: Water

Date Received: 02/28/19 08:00

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,4-Dioxane	2.0	U	2.0	0.86	ug/L			03/02/19 20:13	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	81		63 - 125					03/02/19 20:13	1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 20:53	1
cis-1,2-Dichloroethene	1.0	U	1.0	0.16	ug/L			03/01/19 20:53	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 20:53	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 20:53	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 20:53	1
Vinyl chloride	1.0	U	1.0	0.20	ug/L			03/01/19 20:53	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	89		70 - 121					03/01/19 20:53	1
4-Bromofluorobenzene (Surr)	64		59 - 120					03/01/19 20:53	1
Toluene-d8 (Surr)	72		70 - 123					03/01/19 20:53	1
Dibromofluoromethane (Surr)	89		75 - 128					03/01/19 20:53	1

Client Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-78_022619

Lab Sample ID: 240-108701-5

Date Collected: 02/26/19 16:40

Matrix: Water

Date Received: 02/28/19 08:00

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,4-Dioxane	2.0	U	2.0	0.86	ug/L			03/02/19 20:38	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	82		63 - 125					03/02/19 20:38	1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 21:15	1
cis-1,2-Dichloroethene	0.22	J	1.0	0.16	ug/L			03/01/19 21:15	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 21:15	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 21:15	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 21:15	1
Vinyl chloride	1.0	U	1.0	0.20	ug/L			03/01/19 21:15	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	98		70 - 121					03/01/19 21:15	1
4-Bromofluorobenzene (Surr)	68		59 - 120					03/01/19 21:15	1
Toluene-d8 (Surr)	76		70 - 123					03/01/19 21:15	1
Dibromofluoromethane (Surr)	101		75 - 128					03/01/19 21:15	1

Client Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: TRIP BLANK

Lab Sample ID: 240-108701-6

Date Collected: 02/26/19 00:00

Matrix: Water

Date Received: 02/28/19 08:00

Method: 8260B - Volatile Organic Compounds (GC/MS)

Analyte	Result	Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 21:37	1
cis-1,2-Dichloroethene	1.0	U	1.0	0.16	ug/L			03/01/19 21:37	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 21:37	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 21:37	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 21:37	1
Vinyl chloride	1.0	U	1.0	0.20	ug/L			03/01/19 21:37	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	101		70 - 121		03/01/19 21:37	1
4-Bromofluorobenzene (Surr)	71		59 - 120		03/01/19 21:37	1
Toluene-d8 (Surr)	78		70 - 123		03/01/19 21:37	1
Dibromofluoromethane (Surr)	103		75 - 128		03/01/19 21:37	1

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: ICV 240-364785/14 Calibration Date: 01/21/2019 13:48
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC8416.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Dichlorodifluoromethane	Ave	0.3072	0.3077		0.0100	0.0100	0.2	50.0
Chloromethane	Ave	0.3135	0.2939	0.1000	0.00937	0.0100	-6.3	50.0
Vinyl chloride	Ave	0.2885	0.2965		0.0103	0.0100	2.8	20.0
Butadiene	Ave	0.3794	0.3439		0.00906	0.0100	-9.4	50.0
Bromomethane	Ave	0.2308	0.2181		0.00945	0.0100	-5.5	50.0
Chloroethane	Ave	0.2041	0.1937		0.00949	0.0100	-5.1	50.0
Dichlorofluoromethane	Ave	0.5102	0.5038		0.00987	0.0100	-1.3	50.0
Trichlorofluoromethane	Ave	0.4337	0.4655		0.0107	0.0100	7.3	50.0
Ethyl ether	Ave	0.2310	0.2499		0.0108	0.0100	8.2	50.0
Acrolein	Ave	0.0317	0.0225		0.0354	0.0500	-29.1	50.0
1,1-Dichloroethene	Ave	0.3005	0.2950		0.00982	0.0100	-1.8	20.0
1,1,2-Trichloro-1,2,2-trifluoroethane	Ave	0.2468	0.2669		0.0108	0.0100	8.1	50.0
Acetone	Lin1		0.0260		0.0217	0.0200	8.7	50.0
Iodomethane	Ave	0.4675	0.5088		0.0109	0.0100	8.8	50.0
Carbon disulfide	Ave	0.7741	0.7832		0.0101	0.0100	1.2	50.0
3-Chloro-1-propene	Ave	0.1698	0.1835		0.0108	0.0100	8.0	50.0
Methyl acetate	Ave	0.2050	0.2103		0.0205	0.0200	2.6	50.0
Methylene Chloride	Lin1		0.3143		0.0102	0.0100	1.8	50.0
2-Methyl-2-propanol	Ave	0.0203	0.0193		0.0952	0.100	-4.8	50.0
Acrylonitrile	Ave	0.0962	0.0979		0.102	0.100	1.8	50.0
Methyl tert-butyl ether	Ave	0.7834	0.8124		0.0104	0.0100	3.7	50.0
trans-1,2-Dichloroethene	Ave	0.2795	0.2813		0.0101	0.0100	0.6	50.0
Hexane	Ave	0.0586	0.0579		0.00987	0.0100	-1.3	20.0
1,1-Dichloroethane	Ave	0.4517	0.4658	0.1000	0.0103	0.0100	3.1	50.0
Vinyl acetate	Ave	0.5198	0.5720		0.0110	0.0100	10.0	50.0
2,2-Dichloropropane	Ave	0.0624	0.0692		0.0111	0.0100	10.9	50.0
2-Butanone (MEK)	Ave	0.0333	0.0338		0.0203	0.0200	1.7	50.0
cis-1,2-Dichloroethene	Ave	0.3078	0.3026		0.00983	0.0100	-1.7	50.0
Chlorobromomethane	Ave	0.1531	0.1576		0.0103	0.0100	2.9	50.0
Tetrahydrofuran	Ave	0.0828	0.0821		0.0198	0.0200	-0.8	50.0
Chloroform	Ave	0.4606	0.4715		0.0102	0.0100	2.4	20.0
1,1,1-Trichloroethane	Ave	0.3546	0.3844		0.0108	0.0100	8.4	50.0
Cyclohexane	Ave	0.3993	0.4228		0.0106	0.0100	5.9	50.0
1,1-Dichloropropene	Ave	0.3748	0.3803		0.0101	0.0100	1.5	50.0
Carbon tetrachloride	Ave	0.3441	0.3608		0.0105	0.0100	4.9	50.0
Isobutyl alcohol	Ave	0.0077	0.0075		0.244	0.250	-2.5	50.0
Benzene	Ave	1.116	1.120		0.0100	0.0100	0.4	50.0
1,2-Dichloroethane	Ave	0.3820	0.3923		0.0103	0.0100	2.7	50.0
n-Heptane	Ave	0.0532	0.0516		0.00969	0.0100	-3.1	50.0
Trichloroethene	Ave	0.3240	0.3277		0.0101	0.0100	1.2	50.0

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: ICV 240-364785/14 Calibration Date: 01/21/2019 13:48
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC8416.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Methylcyclohexane	Ave	0.3524	0.3635		0.0103	0.0100	3.1	50.0
1,2-Dichloropropane	Ave	0.2590	0.2693		0.0104	0.0100	4.0	20.0
1,4-Dioxane	Lin1		0.0018		0.174	0.200	-13.1	50.0
Dibromomethane	Ave	0.1717	0.1693		0.00986	0.0100	-1.4	50.0
Dichlorobromomethane	Ave	0.3410	0.3425		0.0100	0.0100	0.5	50.0
2-Chloroethyl vinyl ether	Ave	0.1745	0.1743		0.00998	0.0100	-0.2	50.0
cis-1,3-Dichloropropene	Ave	0.3944	0.4210		0.0107	0.0100	6.7	50.0
4-Methyl-2-pentanone (MIBK)	Ave	0.2678	0.2819		0.0211	0.0200	5.3	50.0
Toluene	Ave	1.476	1.520		0.0103	0.0100	3.0	20.0
trans-1,3-Dichloropropene	Ave	0.4646	0.4706		0.0101	0.0100	1.3	50.0
Ethyl methacrylate	Ave	0.4442	0.4407		0.00992	0.0100	-0.8	50.0
1,1,2-Trichloroethane	Ave	0.2982	0.3097		0.0104	0.0100	3.9	50.0
Tetrachloroethene	Ave	0.3268	0.3359		0.0103	0.0100	2.8	50.0
1,3-Dichloropropane	Ave	0.5243	0.5353		0.0102	0.0100	2.1	50.0
2-Hexanone	Ave	0.2283	0.2452		0.0215	0.0200	7.4	50.0
Chlorodibromomethane	Ave	0.3116	0.3163		0.0102	0.0100	1.5	50.0
Ethylene Dibromide	Ave	0.3191	0.3265		0.0102	0.0100	2.3	50.0
Chlorobenzene	Ave	0.9777	0.9870	0.3000	0.0101	0.0100	1.0	50.0
1,1,1,2-Tetrachloroethane	Ave	0.3450	0.3654		0.0106	0.0100	5.9	50.0
Ethylbenzene	Ave	0.5145	0.5244		0.0102	0.0100	1.9	20.0
m-Xylene & p-Xylene	Ave	1.221	1.254		0.0103	0.0100	2.7	50.0
o-Xylene	Ave	0.6189	0.6401		0.0103	0.0100	3.4	50.0
Styrene	Ave	1.036	1.018		0.00982	0.0100	-1.8	50.0
Bromoform	Lin1		0.1992	0.1000	0.00846	0.0100	-15.4	50.0
Isopropylbenzene	Ave	1.463	1.540		0.0105	0.0100	5.3	50.0
1,1,2,2-Tetrachloroethane	Ave	0.7086	0.7292	0.3000	0.0103	0.0100	2.9	50.0
Bromobenzene	Ave	0.8274	0.8332		0.0101	0.0100	0.7	50.0
1,2,3-Trichloropropane	Ave	0.2468	0.2591		0.0105	0.0100	5.0	50.0
trans-1,4-Dichloro-2-butene	Ave	0.1014	0.0704		0.00695	0.0100	-30.5	50.0
N-Propylbenzene	Ave	0.7286	0.7393		0.0101	0.0100	1.5	50.0
2-Chlorotoluene	Ave	0.6821	0.6987		0.0102	0.0100	2.4	50.0
1,3,5-Trimethylbenzene	Ave	2.119	2.131		0.0101	0.0100	0.6	50.0
4-Chlorotoluene	Ave	2.205	2.165		0.00982	0.0100	-1.8	50.0
tert-Butylbenzene	Ave	1.897	1.872		0.00987	0.0100	-1.3	50.0
1,2,4-Trimethylbenzene	Ave	2.227	2.255		0.0101	0.0100	1.2	50.0
sec-Butylbenzene	Ave	2.327	2.325		0.00999	0.0100	-0.0	50.0
1,3-Dichlorobenzene	Ave	1.425	1.437		0.0101	0.0100	0.9	50.0
4-Isopropyltoluene	Ave	2.083	2.090		0.0100	0.0100	0.3	50.0
1,4-Dichlorobenzene	Ave	1.477	1.484		0.0100	0.0100	0.4	50.0
n-Butylbenzene	Ave	1.649	1.603		0.00972	0.0100	-2.8	50.0
1,2-Dichlorobenzene	Ave	1.387	1.408		0.0102	0.0100	1.5	50.0

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: ICV 240-364785/14 Calibration Date: 01/21/2019 13:48
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC8416.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
1,2-Dibromo-3-Chloropropane	Ave	0.1611	0.1660		0.0103	0.0100	3.0	50.0
1,2,4-Trichlorobenzene	Ave	0.8784	0.8494		0.00967	0.0100	-3.3	50.0
Hexachlorobutadiene	Qua		0.3722		0.00828	0.0100	-17.2	50.0
Naphthalene	Ave	2.209	2.304		0.0104	0.0100	4.3	50.0
1,2,3-Trichlorobenzene	Ave	0.7902	0.7849		0.00993	0.0100	-0.7	50.0
Dibromofluoromethane (Surr)	Ave	0.2366	0.2183		0.00735	0.00797	-7.7	50.0
1,2-Dichloroethane-d4 (Surr)	Ave	0.3042	0.2714		0.00711	0.00797	-10.8	50.0
Toluene-d8 (Surr)	Ave	1.214	1.116		0.00733	0.00797	-8.1	50.0
4-Bromofluorobenzene (Surr)	Ave	0.4341	0.4000		0.00734	0.00797	-7.9	50.0

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8416.D
 Lims ID: ICV
 Client ID:
 Sample Type: ICV
 Inject. Date: 21-Jan-2019 13:48:30 ALS Bottle#: 7 Worklist Smp#: 14
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-014
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist:
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:10:13 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1793251	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	85	1418410	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	796911	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	311994	7.97	7.35	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	387861	7.97	7.11	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	1261093	7.97	7.33	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	96	452132	7.97	7.34	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	551850	10.0	10.0	
10 Chloromethane	50	1.686	1.686	0.000	99	527044	10.0	9.37	
11 Vinyl chloride	62	1.781	1.781	0.000	97	531634	10.0	10.3	
12 Butadiene	54	1.793	1.793	-0.001	96	616742	10.0	9.06	
13 Bromomethane	94	2.053	2.054	-0.001	91	391096	10.0	9.45	
14 Chloroethane	64	2.136	2.137	-0.001	100	347264	10.0	9.49	
15 Dichlorofluoromethane	67	2.302	2.303	-0.001	97	903414	10.0	9.87	
16 Trichlorofluoromethane	101	2.362	2.362	0.000	99	834671	10.0	10.7	
17 Ethyl ether	59	2.575	2.563	0.012	90	448075	10.0	10.8	
18 Acrolein	56	2.694	2.694	0.000	99	201389	50.0	35.4	
19 1,1-Dichloroethene	96	2.789	2.777	0.012	98	529054	10.0	9.82	
20 1,1,2-Trichloro-1,2,2-trif	151	2.800	2.789	0.011	86	478556	10.0	10.8	
22 Acetone	58	2.812	2.812	0.000	100	93357	20.0	21.7	
23 Iodomethane	142	2.931	2.931	0.000	98	912367	10.0	10.9	
24 Carbon disulfide	76	2.990	2.990	0.000	100	1404467	10.0	10.1	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	88	329005	10.0	10.8	
27 Methyl acetate	43	3.085	3.085	0.000	98	754191	20.0	20.5	
28 Methylene Chloride	84	3.180	3.180	0.000	93	563557	10.0	10.2	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	346305	100.0	95.2	
32 Acrylonitrile	53	3.393	3.394	-0.001	99	1755477	100.0	101.8	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	97	504418	10.0	10.1	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	95	1456881	10.0	10.4	
33 Hexane	86	3.619	3.619	0.000	94	103809	10.0	9.87	
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	835310	10.0	10.3	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
36 Vinyl acetate	43	3.785	3.785	0.000	97	1025753	10.0	11.0	
39 cis-1,2-Dichloroethene	96	4.247	4.235	0.012	81	542596	10.0	9.83	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	98	121331	20.0	20.3	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	65	124051	10.0	11.1	
45 Chlorobromomethane	128	4.449	4.449	0.000	88	282681	10.0	10.3	
46 Tetrahydrofuran	42	4.484	4.485	-0.001	86	294586	20.0	19.8	
47 Chloroform	83	4.496	4.496	0.000	93	845575	10.0	10.2	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	98	689257	10.0	10.8	
49 Cyclohexane	56	4.710	4.710	0.000	90	758127	10.0	10.6	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	94	681963	10.0	10.1	
50 Carbon tetrachloride	117	4.805	4.805	0.000	96	647000	10.0	10.5	
52 Isobutyl alcohol	41	4.864	4.864	0.000	95	335938	250.0	243.9	
53 Benzene	78	4.971	4.971	0.000	96	2009249	10.0	10.0	
54 1,2-Dichloroethane	62	4.982	4.983	-0.001	98	703449	10.0	10.3	
56 n-Heptane	100	5.160	5.160	0.000	93	92495	10.0	9.69	
58 Trichloroethene	130	5.504	5.504	0.000	95	587677	10.0	10.1	
60 Methylcyclohexane	83	5.670	5.670	0.000	90	651902	10.0	10.3	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	94	482855	10.0	10.4	
63 Dibromomethane	93	5.813	5.813	0.000	88	303520	10.0	9.86	
64 1,4-Dioxane	88	5.813	5.813	0.000	33	65935	200.0	173.7	
65 Dichlorobromomethane	83	5.931	5.931	0.000	99	614221	10.0	10.0	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	312475	10.0	9.98	
68 cis-1,3-Dichloropropene	75	6.322	6.323	-0.001	95	754933	10.0	10.7	
69 4-Methyl-2-pentanone (MIBK)	43	6.441	6.441	0.000	97	1011196	20.0	21.1	
70 Toluene	91	6.619	6.619	0.000	98	2155730	10.0	10.3	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	94	667505	10.0	10.1	
72 Ethyl methacrylate	69	6.868	6.868	0.000	89	625023	10.0	9.92	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	439234	10.0	10.4	
74 Tetrachloroethene	164	7.117	7.117	0.000	96	476419	10.0	10.3	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	93	759222	10.0	10.2	
76 2-Hexanone	43	7.188	7.188	0.000	97	695520	20.0	21.5	
79 Chlorodibromomethane	129	7.342	7.342	0.000	89	448610	10.0	10.2	
80 Ethylene Dibromide	107	7.461	7.461	0.000	98	463121	10.0	10.2	
82 Chlorobenzene	112	7.900	7.900	0.000	95	1399979	10.0	10.1	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	94	518307	10.0	10.6	
84 Ethylbenzene	106	7.995	7.995	-0.001	98	743771	10.0	10.2	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	1778779	10.0	10.3	
86 o-Xylene	106	8.481	8.481	0.000	95	907873	10.0	10.3	
87 Styrene	104	8.493	8.493	0.000	94	1443373	10.0	9.82	
88 Bromoform	173	8.682	8.682	0.000	98	282491	10.0	8.46	
89 Isopropylbenzene	105	8.825	8.825	0.000	95	2184869	10.0	10.5	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	581082	10.0	10.3	
92 Bromobenzene	156	9.133	9.133	0.000	91	663996	10.0	10.1	
95 trans-1,4-Dichloro-2-buten	53	9.168	9.169	-0.001	67	56124	10.0	6.95	
94 1,2,3-Trichloropropane	110	9.168	9.169	-0.001	84	206463	10.0	10.5	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	589187	10.0	10.1	
97 2-Chlorotoluene	126	9.323	9.323	0.000	97	556828	10.0	10.2	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	1698481	10.0	10.1	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	1725613	10.0	9.82	
101 tert-Butylbenzene	119	9.714	9.714	0.000	92	1491725	10.0	9.87	
103 1,2,4-Trimethylbenzene	105	9.761	9.762	-0.001	94	1796823	10.0	10.1	
105 sec-Butylbenzene	105	9.927	9.928	-0.001	94	1852982	10.0	10.0	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	98	1145305	10.0	10.1	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	97	1665303	10.0	10.0	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	96	1182487	10.0	10.0	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	1277066	10.0	9.72	
112 1,2-Dichlorobenzene	146	10.509	10.509	-0.001	99	1122403	10.0	10.2	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	89	132296	10.0	10.3	
115 1,2,4-Trichlorobenzene	180	12.109	12.110	-0.001	94	676924	10.0	9.67	
116 Hexachlorobutadiene	225	12.275	12.276	-0.001	93	296600	10.0	8.28	
117 Naphthalene	128	12.358	12.359	-0.001	96	1836241	10.0	10.4	
118 1,2,3-Trichlorobenzene	180	12.607	12.608	-0.001	95	625482	10.0	9.93	
S 129 Xylenes, Total	106				0		20.0	20.6	
S 157 Total BTEX	1		0.000				50.0	ND	
S 130 Trihalomethanes, Total	1				0		40.0	38.9	

Reagents:

VMFASPW_00285	Amount Added: 8.00	Units: uL	
VMFASAW_00264	Amount Added: 8.00	Units: uL	
VMFASGW_00293	Amount Added: 8.00	Units: uL	
VM50IS_00072	Amount Added: 1.00	Units: uL	
vmDist_H2o_00124	Amount Added: 0.00	Units:	Run Reagent
vm50ss_stk_00079	Amount Added: 0.80	Units: uL	Run Reagent

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8416.D

Injection Date: 21-Jan-2019 13:48:30

Instrument ID: A3UX15

Operator ID:

Lims ID: ICV

Worklist Smp#: 14

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 7

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

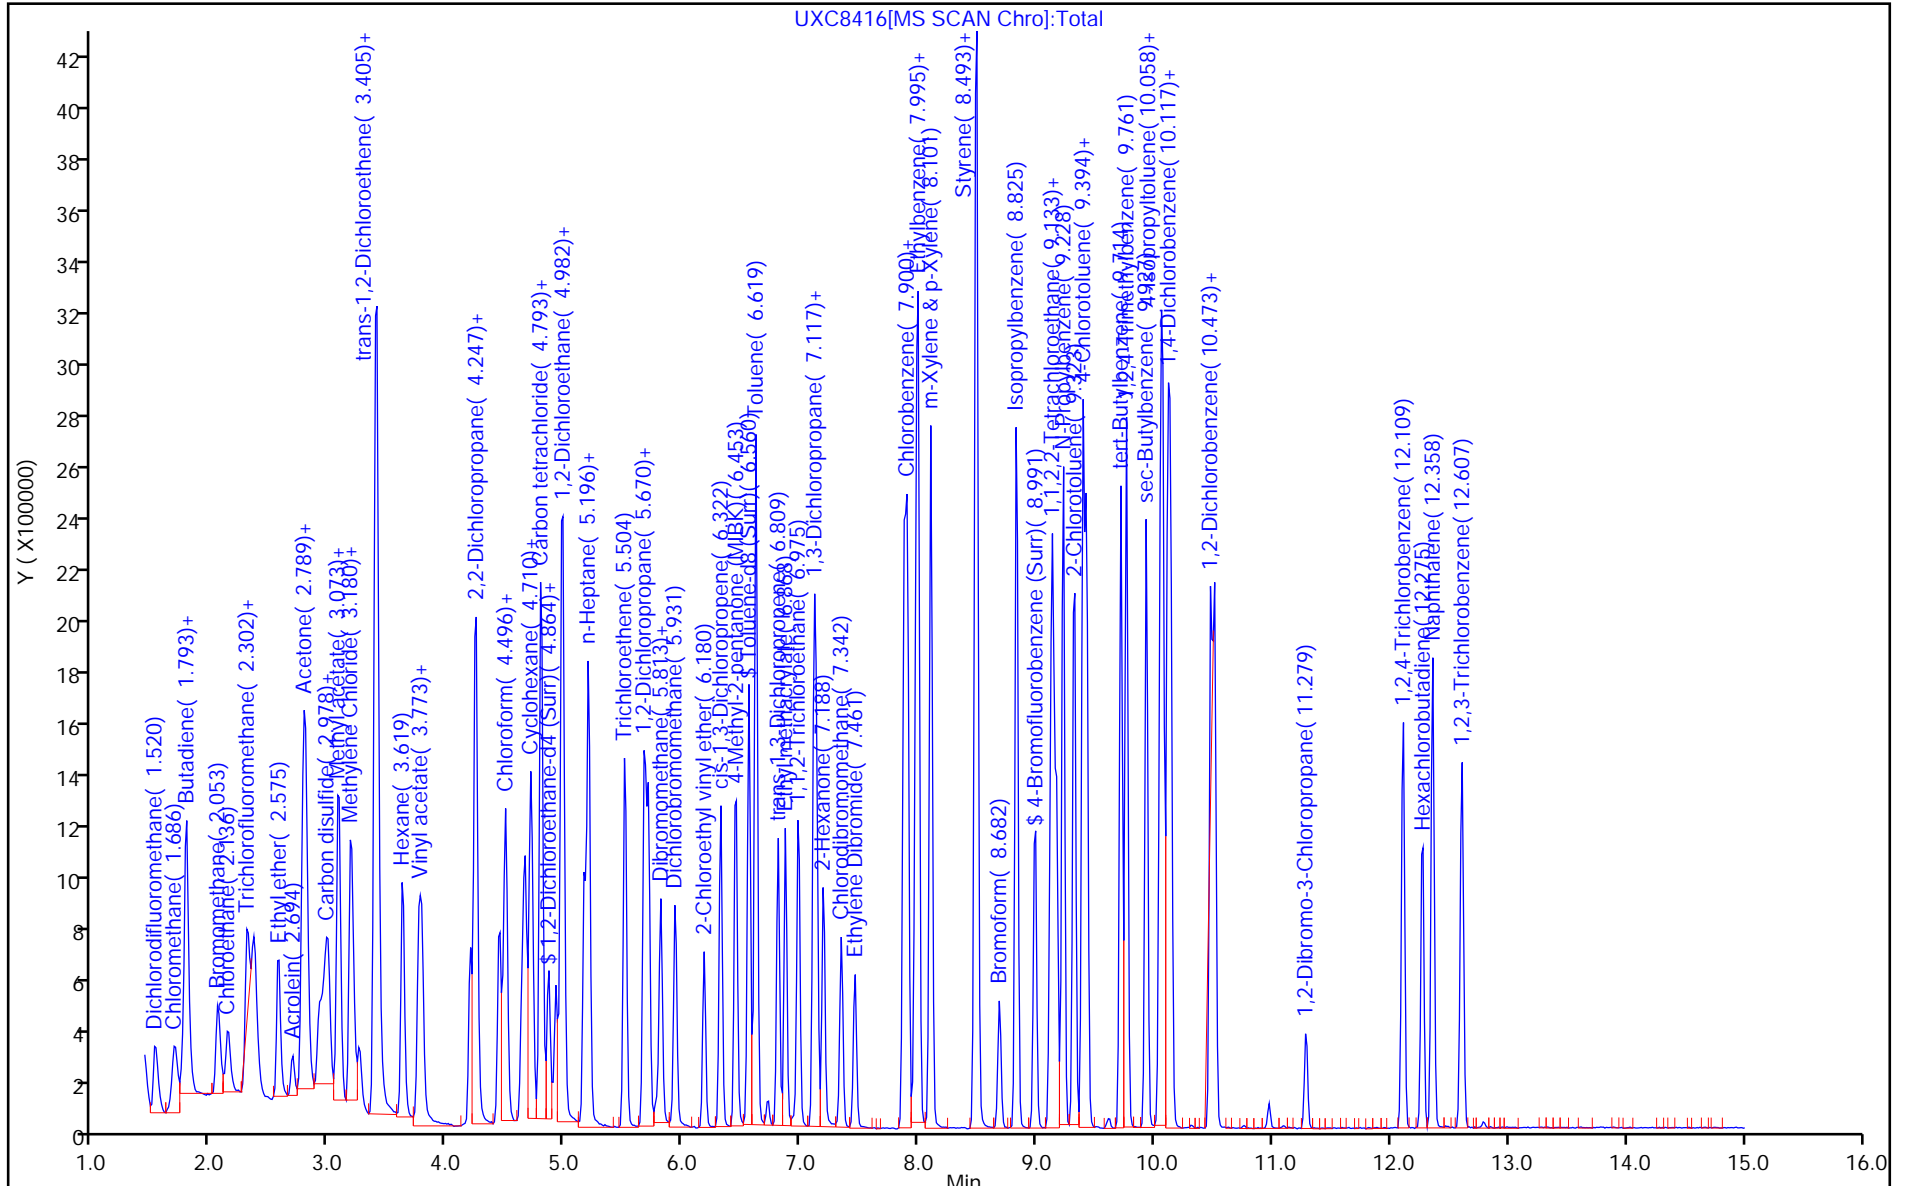

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: ICV 240-364785/15 Calibration Date: 01/21/2019 16:21
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC8423.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Dibromofluoromethane (Surr)	Ave	0.2366	0.2218		0.00747	0.00797	-6.3	50.0
1,2-Dichloroethane-d4 (Surr)	Ave	0.3042	0.2777		0.00728	0.00797	-8.7	50.0
Toluene-d8 (Surr)	Ave	1.214	1.132		0.00743	0.00797	-6.7	50.0
4-Bromofluorobenzene (Surr)	Ave	0.4341	0.4058		0.00745	0.00797	-6.5	50.0

TestAmerica Canton
Target Compound Quantitation Report


Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8423.D
 Lims ID: ICV A9
 Client ID:
 Sample Type: ICV
 Inject. Date: 21-Jan-2019 16:21:30 ALS Bottle#: 14 Worklist Smp#: 15
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-015
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist:
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:10:13 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1778453	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	85	1420097	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	764446	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	314414	7.97	7.47	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	393596	7.97	7.28	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	1281042	7.97	7.43	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	97	459309	7.97	7.45	
26 Acetonitrile	41	3.061	3.050	0.011	98	427448	100.0	104.0	
35 Isopropyl ether	87	3.797	3.797	0.000	92	442161	10.0	10.3	
37 2-Chloro-1,3-butadiene	53	3.832	3.832	0.000	93	736814	10.0	9.78	
38 Tert-butyl ethyl ether	59	4.093	4.093	0.000	97	1388893	10.0	10.0	
42 Ethyl acetate	43	4.283	4.283	0.000	99	937785	20.0	20.8	
43 Propionitrile	54	4.307	4.307	0.000	99	677621	100.0	106.8	
44 Methacrylonitrile	41	4.437	4.425	0.012	92	3212963	100.0	104.3	
55 Tert-amyl methyl ether	73	5.054	5.042	0.012	98	1404415	10.0	10.2	
57 n-Butanol	56	5.421	5.421	0.000	89	269615	250.0	249.7	
59 Ethyl acrylate	55	5.575	5.575	0.000	99	624490	10.0	10.5	
62 Methyl methacrylate	41	5.777	5.777	0.000	91	913802	20.0	21.1	
66 2-Nitropropane	41	6.133	6.133	0.000	99	271968	20.0	20.5	
77 n-Butyl acetate	43	7.295	7.295	0.000	97	736671	10.0	10.6	
81 1-Chlorohexane	91	7.864	7.864	0.000	98	551389	10.0	9.79	
91 Cyclohexanone	55	8.943	8.931	0.012	94	139432	100.0	114.7	
102 Pentachloroethane	167	9.750	9.750	0.000	95	563326	20.0	19.5	
109 1,2,3-Trimethylbenzene	105	10.176	10.176	0.000	98	1800683	10.0	10.3	
110 Benzyl chloride	126	10.271	10.271	0.000	98	227669	10.0	10.1	
114 1,3,5-Trichlorobenzene	180	11.493	11.493	0.000	97	692380	10.0	9.57	
119 2-Methylnaphthalene	142	13.651	13.651	0.000	93	1419962	20.0	17.3	

Reagents:

VMFASA9W_00216	Amount Added: 8.00	Units: uL	
VM50IS_00072	Amount Added: 1.00	Units: uL	
vmDist_H2o_00124	Amount Added: 0.00	Units:	Run Reagent
vm50ss_stk_00079	Amount Added: 0.80	Units: uL	Run Reagent

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

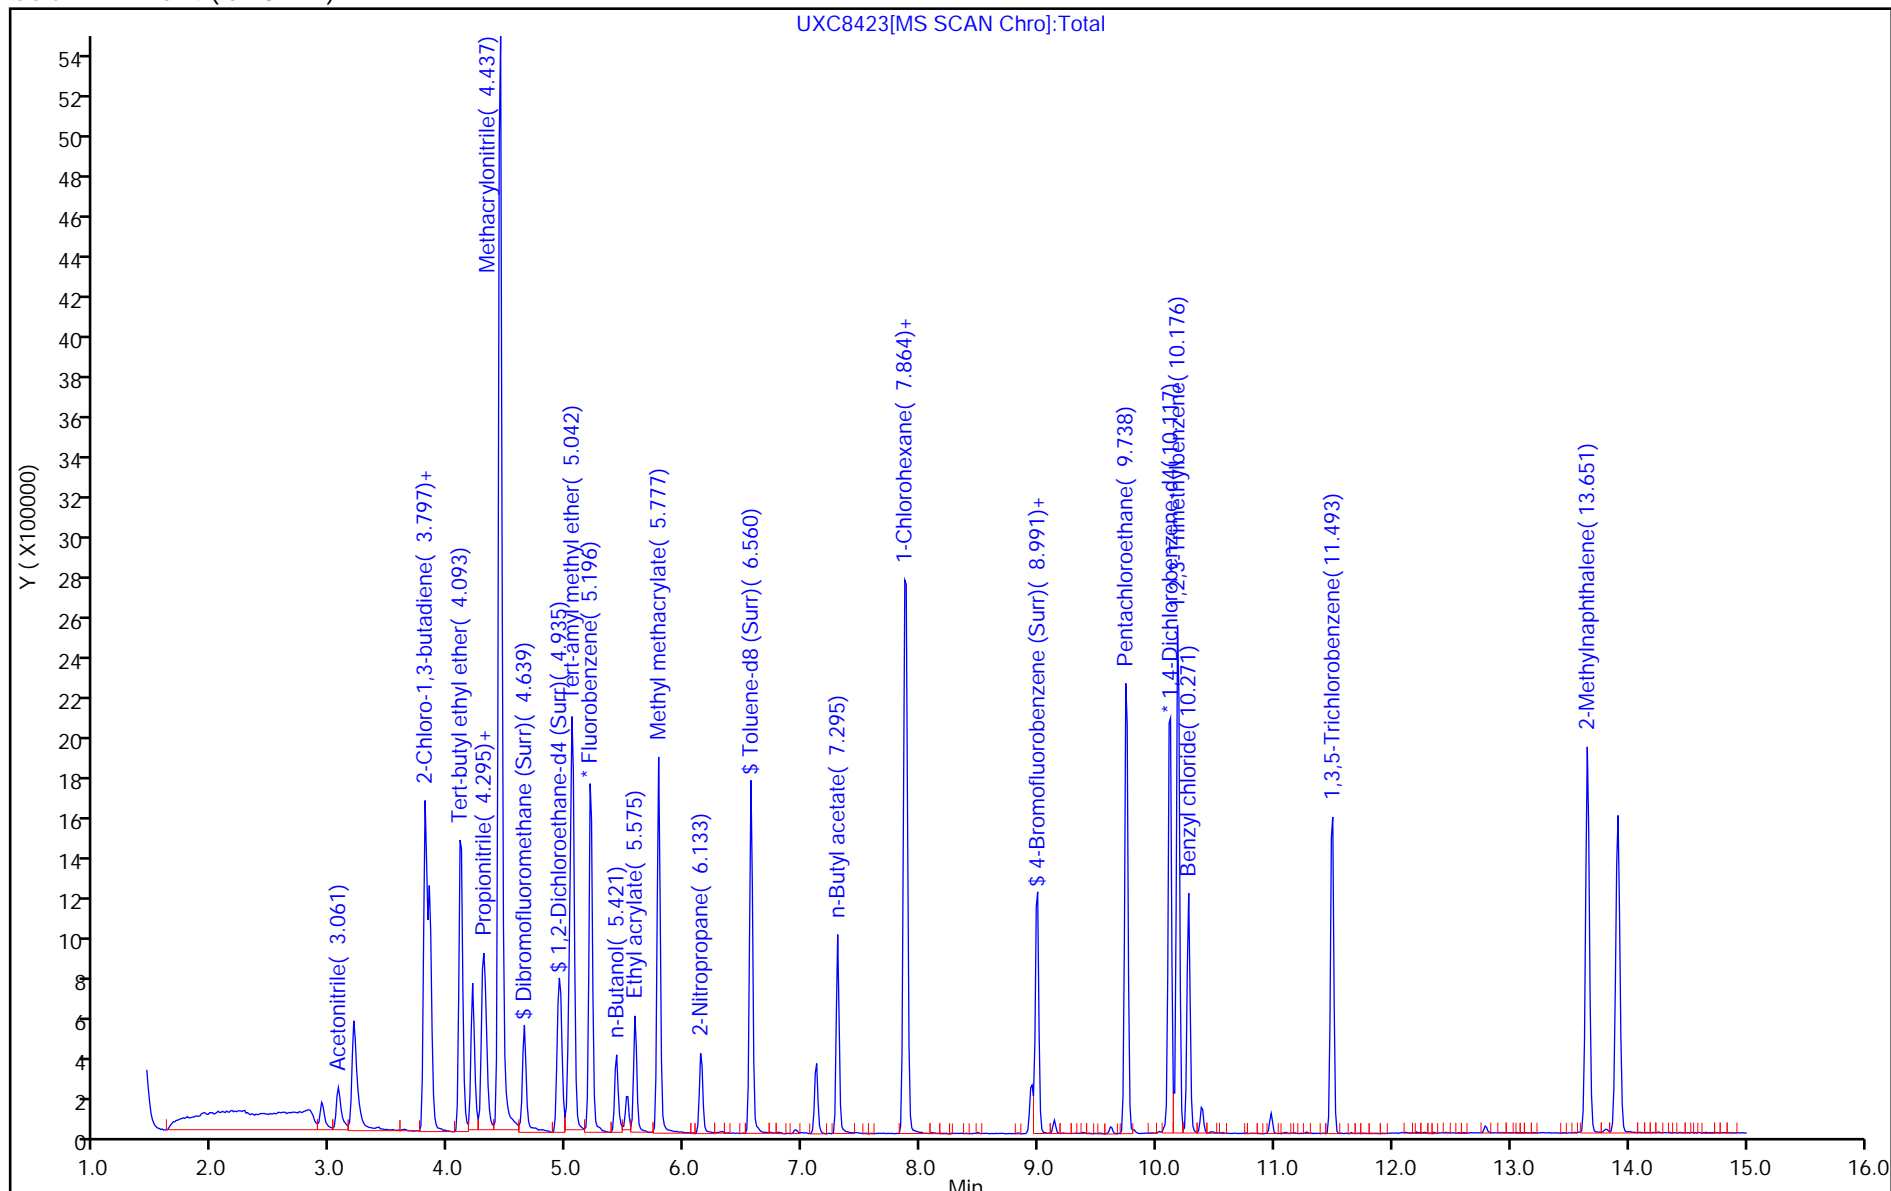

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: ICV 240-364785/15 Calibration Date: 01/21/2019 16:21
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 14:10
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 15:59
 Lab File ID: UXC8423.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Acetonitrile	Ave	0.0231	0.0240		0.104	0.100	4.0	50.0
Isopropyl ether	Ave	0.2405	0.2486		0.0103	0.0100	3.4	50.0
2-Chloro-1,3-butadiene	Ave	0.4235	0.4143		0.00978	0.0100	-2.2	50.0
Tert-butyl ethyl ether	Ave	0.7799	0.7810		0.0100	0.0100	0.1	50.0
Ethyl acetate	Ave	0.2538	0.2637		0.0208	0.0200	3.9	50.0
Propionitrile	Ave	0.0357	0.0381		0.107	0.100	6.8	50.0
Methacrylonitrile	Ave	0.1733	0.1807		0.104	0.100	4.3	50.0
Tert-amyl methyl ether	Ave	0.7765	0.7897		0.0102	0.0100	1.7	50.0
n-Butanol	Ave	0.0061	0.0061		0.250	0.250	-0.1	50.0
Ethyl acrylate	Ave	0.3330	0.3511		0.0105	0.0100	5.4	50.0
Methyl methacrylate	Ave	0.2430	0.2569		0.0211	0.0200	5.7	50.0
2-Nitropropane	Ave	0.0745	0.0765		0.0205	0.0200	2.7	50.0
n-Butyl acetate	Ave	0.3918	0.4142		0.0106	0.0100	5.7	50.0
1-Chlorohexane	Ave	0.3968	0.3883		0.00979	0.0100	-2.1	50.0
Cyclohexanone	Lin1		0.0182		0.115	0.100	14.7	50.0
Pentachloroethane	Ave	0.2034	0.1983		0.0195	0.0200	-2.5	50.0
1,2,3-Trimethylbenzene	Ave	2.297	2.356		0.0103	0.0100	2.5	50.0
Benzyl chloride	Ave	0.2963	0.2978		0.0101	0.0100	0.5	50.0
1,3,5-Trichlorobenzene	Ave	0.9466	0.9057		0.00957	0.0100	-4.3	50.0
2-Methylnaphthalene	Ave	1.076	0.9288		0.0173	0.0200	-13.7	50.0

TestAmerica Canton
Target Compound Quantitation Report


Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8423.D
 Lims ID: ICV A9
 Client ID:
 Sample Type: ICV
 Inject. Date: 21-Jan-2019 16:21:30 ALS Bottle#: 14 Worklist Smp#: 15
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-015
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist:
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:10:13 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1778453	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	85	1420097	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	764446	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	314414	7.97	7.47	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	393596	7.97	7.28	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	1281042	7.97	7.43	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	97	459309	7.97	7.45	
26 Acetonitrile	41	3.061	3.050	0.011	98	427448	100.0	104.0	
35 Isopropyl ether	87	3.797	3.797	0.000	92	442161	10.0	10.3	
37 2-Chloro-1,3-butadiene	53	3.832	3.832	0.000	93	736814	10.0	9.78	
38 Tert-butyl ethyl ether	59	4.093	4.093	0.000	97	1388893	10.0	10.0	
42 Ethyl acetate	43	4.283	4.283	0.000	99	937785	20.0	20.8	
43 Propionitrile	54	4.307	4.307	0.000	99	677621	100.0	106.8	
44 Methacrylonitrile	41	4.437	4.425	0.012	92	3212963	100.0	104.3	
55 Tert-amyl methyl ether	73	5.054	5.042	0.012	98	1404415	10.0	10.2	
57 n-Butanol	56	5.421	5.421	0.000	89	269615	250.0	249.7	
59 Ethyl acrylate	55	5.575	5.575	0.000	99	624490	10.0	10.5	
62 Methyl methacrylate	41	5.777	5.777	0.000	91	913802	20.0	21.1	
66 2-Nitropropane	41	6.133	6.133	0.000	99	271968	20.0	20.5	
77 n-Butyl acetate	43	7.295	7.295	0.000	97	736671	10.0	10.6	
81 1-Chlorohexane	91	7.864	7.864	0.000	98	551389	10.0	9.79	
91 Cyclohexanone	55	8.943	8.931	0.012	94	139432	100.0	114.7	
102 Pentachloroethane	167	9.750	9.750	0.000	95	563326	20.0	19.5	
109 1,2,3-Trimethylbenzene	105	10.176	10.176	0.000	98	1800683	10.0	10.3	
110 Benzyl chloride	126	10.271	10.271	0.000	98	227669	10.0	10.1	
114 1,3,5-Trichlorobenzene	180	11.493	11.493	0.000	97	692380	10.0	9.57	
119 2-Methylnaphthalene	142	13.651	13.651	0.000	93	1419962	20.0	17.3	

Reagents:

VMFASA9W_00216	Amount Added: 8.00	Units: uL	
VM50IS_00072	Amount Added: 1.00	Units: uL	
vmDist_H2o_00124	Amount Added: 0.00	Units:	Run Reagent
vm50ss_stk_00079	Amount Added: 0.80	Units: uL	Run Reagent

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

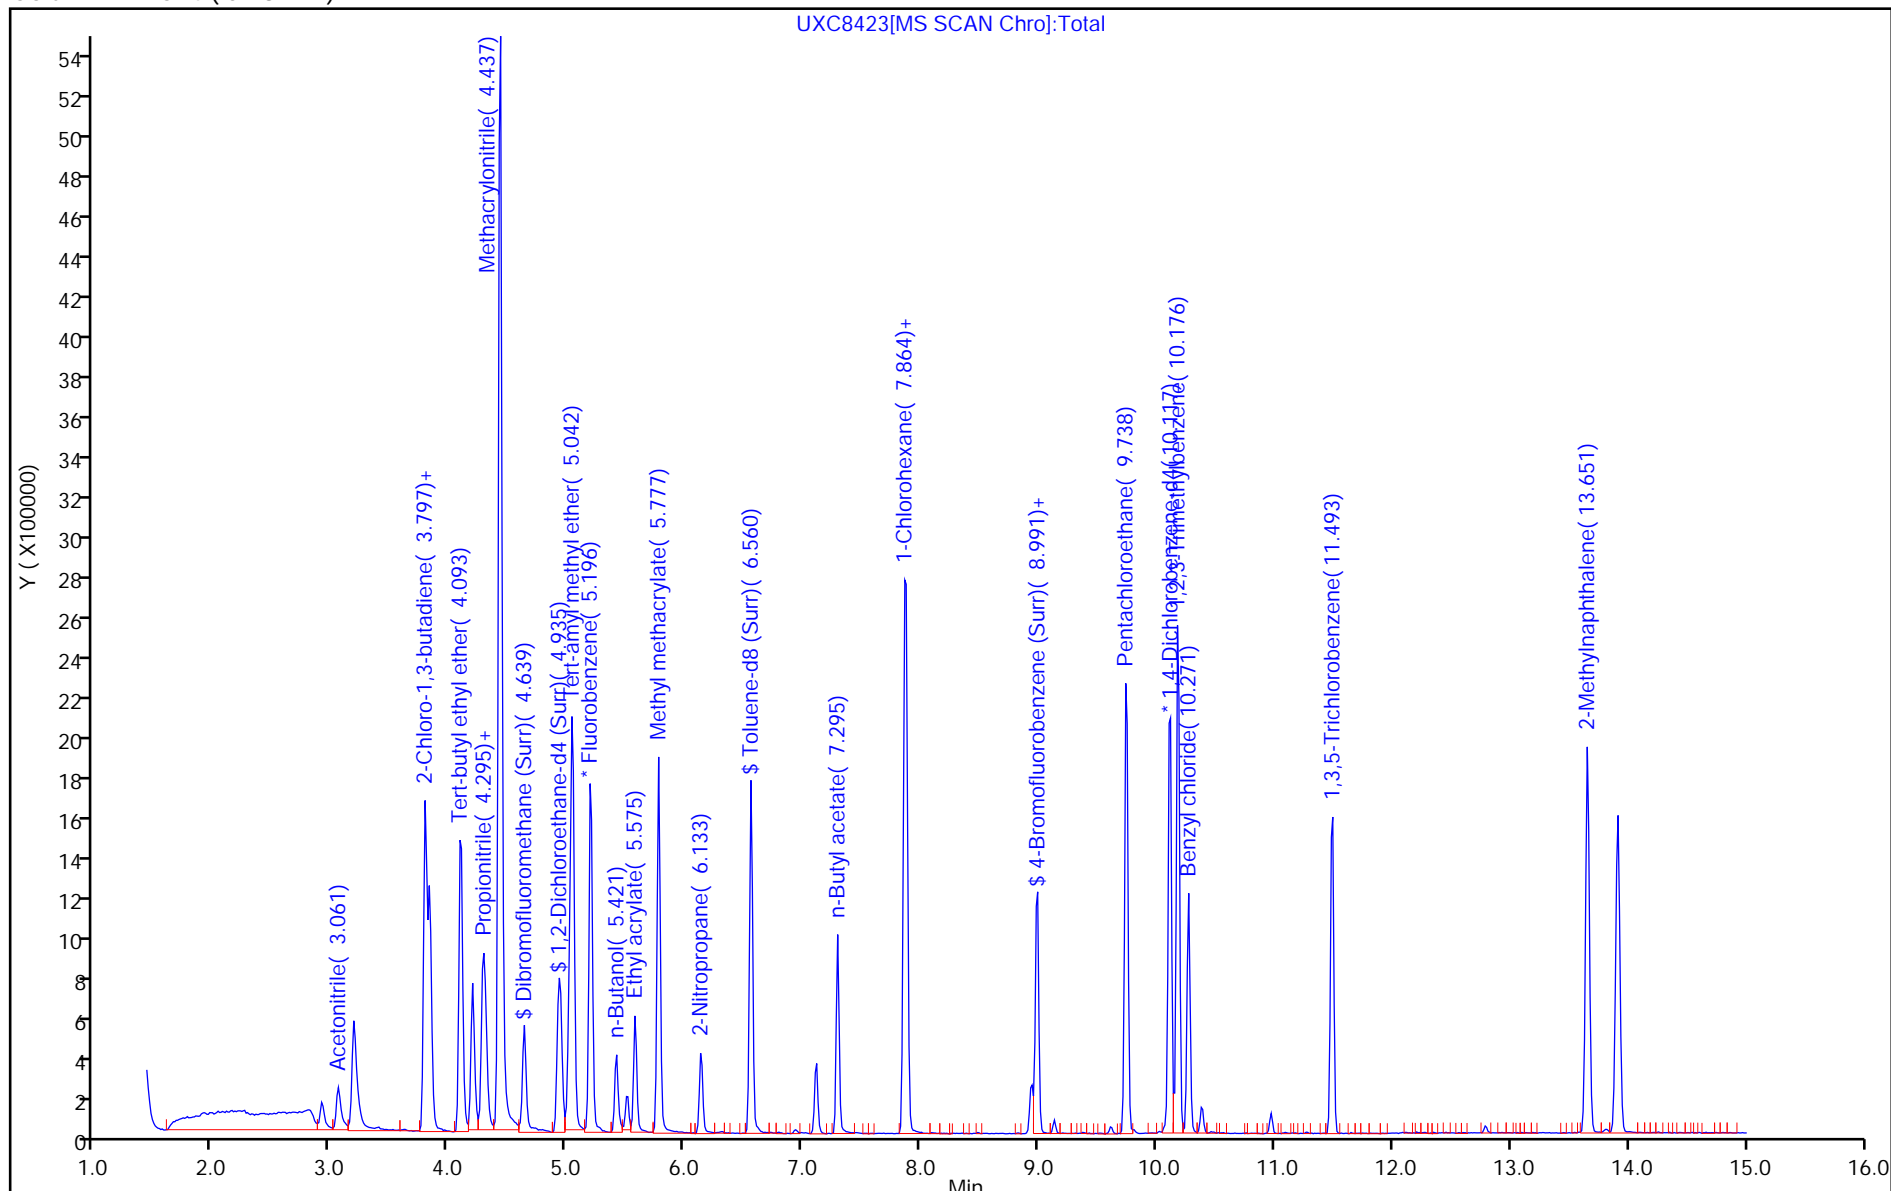

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: CCVIS 240-369935/2 Calibration Date: 03/01/2019 11:33
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC9085.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Dichlorodifluoromethane	Ave	0.3072	0.3140		0.0102	0.0100	2.2	50.0
Chloromethane	Ave	0.3135	0.2882	0.1000	0.00919	0.0100	-8.1	50.0
Vinyl chloride	Ave	0.2885	0.2896		0.0100	0.0100	0.4	20.0
Butadiene	Ave	0.3794	0.3237		0.00853	0.0100	-14.7	50.0
Bromomethane	Ave	0.2308	0.2211		0.00958	0.0100	-4.2	50.0
Chloroethane	Ave	0.2041	0.1956		0.00958	0.0100	-4.2	50.0
Dichlorofluoromethane	Ave	0.5102	0.4660		0.00913	0.0100	-8.7	50.0
Trichlorofluoromethane	Ave	0.4337	0.5007		0.0115	0.0100	15.5	50.0
Ethyl ether	Ave	0.2310	0.2106		0.00912	0.0100	-8.8	50.0
Acrolein	Ave	0.0317	0.0329		0.0519	0.0500	3.9	50.0
1,1-Dichloroethene	Ave	0.3005	0.2768		0.00921	0.0100	-7.9	20.0
1,1,2-Trichloro-1,2,2-trifluoroethane	Ave	0.2468	0.2741		0.0111	0.0100	11.1	50.0
Acetone	Lin1		0.0215		0.0176	0.0200	-12.2	50.0
Iodomethane	Ave	0.4675	0.5217		0.0112	0.0100	11.6	50.0
Carbon disulfide	Ave	0.7741	0.6259		0.00809	0.0100	-19.1	50.0
3-Chloro-1-propene	Ave	0.1698	0.1579		0.00929	0.0100	-7.1	50.0
Methyl acetate	Ave	0.2050	0.1459		0.0142	0.0200	-28.9	50.0
Methylene Chloride	Lin1		0.3328		0.0109	0.0100	9.3	50.0
2-Methyl-2-propanol	Ave	0.0203	0.0117		0.0577	0.100	-42.3	50.0
Acrylonitrile	Ave	0.0962	0.0783		0.0815	0.100	-18.5	50.0
Methyl tert-butyl ether	Ave	0.7834	0.6030		0.00770	0.0100	-23.0	50.0
trans-1,2-Dichloroethene	Ave	0.2795	0.3096		0.0111	0.0100	10.8	50.0
Hexane	Ave	0.0586	0.0544		0.00928	0.0100	-7.2	20.0
1,1-Dichloroethane	Ave	0.4517	0.4820	0.1000	0.0107	0.0100	6.7	50.0
Vinyl acetate	Ave	0.5198	0.3392		0.00653	0.0100	-34.7	50.0
cis-1,2-Dichloroethene	Ave	0.3078	0.3423		0.0111	0.0100	11.2	50.0
2,2-Dichloropropane	Ave	0.0624	0.0633		0.0101	0.0100	1.5	50.0
2-Butanone (MEK)	Ave	0.0333	0.0246		0.0148	0.0200	-26.0	50.0
Chlorobromomethane	Ave	0.1531	0.1742		0.0114	0.0100	13.8	50.0
Tetrahydrofuran	Ave	0.0828	0.0520		0.0126	0.0200	-37.2	50.0
Chloroform	Ave	0.4606	0.5178		0.0112	0.0100	12.4	20.0
1,1,1-Trichloroethane	Ave	0.3546	0.4046		0.0114	0.0100	14.1	50.0
Cyclohexane	Ave	0.3993	0.3848		0.00964	0.0100	-3.6	50.0
1,1-Dichloropropene	Ave	0.3748	0.3838		0.0102	0.0100	2.4	50.0
Carbon tetrachloride	Ave	0.3441	0.3496		0.0102	0.0100	1.6	50.0
Isobutyl alcohol	Ave	0.0077	0.0049		0.158	0.250	-36.9	50.0
Benzene	Ave	1.116	1.219		0.0109	0.0100	9.2	50.0
1,2-Dichloroethane	Ave	0.3820	0.3992		0.0105	0.0100	4.5	50.0
n-Heptane	Ave	0.0532	0.0484		0.00909	0.0100	-9.1	50.0
Trichloroethene	Ave	0.3240	0.3646		0.0113	0.0100	12.5	50.0

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: CCVIS 240-369935/2 Calibration Date: 03/01/2019 11:33
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC9085.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Methylcyclohexane	Ave	0.3524	0.3489		0.00990	0.0100	-1.0	50.0
1,2-Dichloropropane	Ave	0.2590	0.2557		0.00987	0.0100	-1.3	20.0
1,4-Dioxane	Lin1		0.0022		0.208	0.200	4.0	50.0
Dibromomethane	Ave	0.1717	0.1657		0.00965	0.0100	-3.5	50.0
Dichlorobromomethane	Ave	0.3410	0.3182		0.00933	0.0100	-6.7	50.0
2-Chloroethyl vinyl ether	Ave	0.1745	0.1082		0.0124	0.0200	-38.0	50.0
cis-1,3-Dichloropropene	Ave	0.3944	0.3150		0.00799	0.0100	-20.1	50.0
4-Methyl-2-pentanone (MIBK)	Ave	0.2678	0.1602		0.0120	0.0200	-40.2	50.0
Toluene	Ave	1.476	1.372		0.00929	0.0100	-7.1	20.0
trans-1,3-Dichloropropene	Ave	0.4646	0.2812		0.00605	0.0100	-39.5	50.0
Ethyl methacrylate	Ave	0.4442	0.2504		0.00564	0.0100	-43.6	50.0
1,1,2-Trichloroethane	Ave	0.2982	0.2473		0.00829	0.0100	-17.1	50.0
Tetrachloroethene	Ave	0.3268	0.3387		0.0104	0.0100	3.7	50.0
1,3-Dichloropropane	Ave	0.5243	0.4216		0.00804	0.0100	-19.6	50.0
2-Hexanone	Ave	0.2283	0.1209		0.0106	0.0200	-47.0	50.0
Chlorodibromomethane	Ave	0.3116	0.2342		0.00752	0.0100	-24.8	50.0
Ethylene Dibromide	Ave	0.3191	0.2419		0.00758	0.0100	-24.2	50.0
Chlorobenzene	Ave	0.9777	0.9096	0.3000	0.00930	0.0100	-7.0	50.0
1,1,1,2-Tetrachloroethane	Ave	0.3450	0.3086		0.00894	0.0100	-10.6	50.0
Ethylbenzene	Ave	0.5145	0.4584		0.00891	0.0100	-10.9	20.0
m-Xylene & p-Xylene	Ave	1.221	1.100		0.00901	0.0100	-9.9	50.0
o-Xylene	Ave	0.6189	0.5747		0.00929	0.0100	-7.1	50.0
Styrene	Ave	1.036	0.9433		0.00911	0.0100	-8.9	50.0
Bromoform	Lin1		0.1265	0.1000	0.00560	0.0100	-44.0	50.0
Isopropylbenzene	Ave	1.463	1.325		0.00906	0.0100	-9.4	50.0
1,1,2,2-Tetrachloroethane	Ave	0.7086	0.4508	0.3000	0.00636	0.0100	-36.4	50.0
Bromobenzene	Ave	0.8274	0.7074		0.00855	0.0100	-14.5	50.0
1,2,3-Trichloropropane	Ave	0.2468	0.1639		0.00664	0.0100	-33.6	50.0
trans-1,4-Dichloro-2-butene	Ave	0.1014	0.0721		0.00711	0.0100	-28.9	50.0
N-Propylbenzene	Ave	0.7286	0.5990		0.00822	0.0100	-17.8	50.0
2-Chlorotoluene	Ave	0.6821	0.5713		0.00838	0.0100	-16.2	50.0
1,3,5-Trimethylbenzene	Ave	2.119	1.798		0.00849	0.0100	-15.1	50.0
4-Chlorotoluene	Ave	2.205	1.814		0.00822	0.0100	-17.8	50.0
tert-Butylbenzene	Ave	1.897	1.516		0.00799	0.0100	-20.1	50.0
1,2,4-Trimethylbenzene	Ave	2.227	1.930		0.00866	0.0100	-13.4	50.0
sec-Butylbenzene	Ave	2.327	1.889		0.00812	0.0100	-18.8	50.0
1,3-Dichlorobenzene	Ave	1.425	1.252		0.00879	0.0100	-12.1	50.0
4-Isopropyltoluene	Ave	2.083	1.739		0.00835	0.0100	-16.5	50.0
1,4-Dichlorobenzene	Ave	1.477	1.292		0.00875	0.0100	-12.5	50.0
n-Butylbenzene	Ave	1.649	1.262		0.00766	0.0100	-23.4	50.0
1,2-Dichlorobenzene	Ave	1.387	1.237		0.00892	0.0100	-10.8	50.0

FORM VII
GC/MS VOA CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Lab Sample ID: CCVIS 240-369935/2 Calibration Date: 03/01/2019 11:33
 Instrument ID: A3UX15 Calib Start Date: 01/21/2019 11:37
 GC Column: DB-624 ID: 0.18 (mm) Calib End Date: 01/21/2019 13:26
 Lab File ID: UXC9085.D Conc. Units: ng/uL Heated Purge: (Y/N) N

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
1,2-Dibromo-3-Chloropropane	Ave	0.1611	0.0672		0.00417	0.0100	-58.3*	50.0
1,2,4-Trichlorobenzene	Ave	0.8784	0.6867		0.00782	0.0100	-21.8	50.0
Hexachlorobutadiene	Qua		0.3455		0.00764	0.0100	-23.6	50.0
Naphthalene	Ave	2.209	1.244		0.00563	0.0100	-43.7	50.0
1,2,3-Trichlorobenzene	Ave	0.7902	0.6379		0.00807	0.0100	-19.3	50.0
Dibromofluoromethane (Surr)	Ave	0.2366	0.2154		0.00726	0.00797	-9.0	50.0
1,2-Dichloroethane-d4 (Surr)	Ave	0.3042	0.2559		0.00670	0.00797	-15.9	50.0
Toluene-d8 (Surr)	Ave	1.214	0.9390		0.00617	0.00797	-22.6	50.0
4-Bromofluorobenzene (Surr)	Ave	0.4341	0.3289		0.00604	0.00797	-24.2	50.0

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9085.D
 Lims ID: CCVIS L4 8260
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 01-Mar-2019 11:33:30 ALS Bottle#: 1 Worklist Smp#: 2
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-002
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:10 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1623662	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	88	1433575	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	92	895002	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	278763	7.97	7.26	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	331088	7.97	6.70	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	1072852	7.97	6.17	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	95	375765	7.97	6.04	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	509860	10.0	10.2	
10 Chloromethane	50	1.686	1.686	0.000	99	467868	10.0	9.19	
11 Vinyl chloride	62	1.781	1.781	0.000	98	470262	10.0	10.0	
12 Butadiene	54	1.793	1.793	0.000	98	525589	10.0	8.53	
13 Bromomethane	94	2.053	2.053	0.000	90	359041	10.0	9.58	
14 Chloroethane	64	2.136	2.136	0.000	100	317617	10.0	9.58	
15 Dichlorofluoromethane	67	2.302	2.302	0.000	97	756648	10.0	9.13	
16 Trichlorofluoromethane	101	2.350	2.350	0.000	99	812904	10.0	11.5	
17 Ethyl ether	59	2.563	2.563	0.000	89	341912	10.0	9.12	
18 Acrolein	56	2.682	2.682	0.000	99	267361	50.0	51.9	
19 1,1-Dichloroethene	96	2.777	2.777	0.000	98	449418	10.0	9.21	
20 1,1,2-Trichloro-1,2,2-trif	151	2.789	2.789	0.000	85	445046	10.0	11.1	
22 Acetone	58	2.812	2.812	0.000	100	69849	20.0	17.6	
23 Iodomethane	142	2.907	2.907	0.000	97	847132	10.0	11.2	
24 Carbon disulfide	76	2.978	2.978	0.000	99	1016279	10.0	8.09	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	89	256287	10.0	9.29	
27 Methyl acetate	43	3.085	3.085	0.000	97	473699	20.0	14.2	
28 Methylene Chloride	84	3.180	3.180	0.000	90	540403	10.0	10.9	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	90	189947	100.0	57.7	
32 Acrylonitrile	53	3.393	3.393	0.000	99	1271887	100.0	81.5	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	979001	10.0	7.70	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	96	502720	10.0	11.1	
33 Hexane	86	3.619	3.619	0.000	94	88382	10.0	9.28	
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	782647	10.0	10.7	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
36 Vinyl acetate	43	3.785	3.785	0.000	97	550798	10.0	6.53	
39 cis-1,2-Dichloroethene	96	4.235	4.235	0.000	80	555749	10.0	11.1	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	98	79875	20.0	14.8	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	64	102793	10.0	10.1	
45 Chlorobromomethane	128	4.449	4.449	0.000	87	282895	10.0	11.4	
46 Tetrahydrofuran	42	4.484	4.484	0.000	87	168909	20.0	12.6	
47 Chloroform	83	4.496	4.496	0.000	93	840700	10.0	11.2	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	99	656893	10.0	11.4	
49 Cyclohexane	56	4.710	4.710	0.000	88	624728	10.0	9.64	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	95	623115	10.0	10.2	
50 Carbon tetrachloride	117	4.805	4.805	0.000	96	567579	10.0	10.2	
52 Isobutyl alcohol	41	4.864	4.864	0.000	92	196902	250.0	157.9	
53 Benzene	78	4.971	4.971	0.000	95	1979023	10.0	10.9	
54 1,2-Dichloroethane	62	4.982	4.982	0.000	98	648226	10.0	10.5	
56 n-Heptane	100	5.172	5.172	0.000	88	78508	10.0	9.09	
58 Trichloroethene	130	5.504	5.504	0.000	95	591944	10.0	11.3	
60 Methylcyclohexane	83	5.670	5.670	0.000	89	566452	10.0	9.90	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	94	415151	10.0	9.87	
63 Dibromomethane	93	5.813	5.813	0.000	87	269102	10.0	9.65	
64 1,4-Dioxane	88	5.813	5.813	0.000	89	71903	200.0	208.1	
65 Dichlorobromomethane	83	5.931	5.931	0.000	99	516710	10.0	9.33	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	94	351237	20.0	12.4	
68 cis-1,3-Dichloropropene	75	6.322	6.322	0.000	95	511461	10.0	7.99	
69 4-Methyl-2-pentanone (MIBK)	43	6.453	6.453	0.000	96	520115	20.0	12.0	
70 Toluene	91	6.619	6.619	0.000	98	1966957	10.0	9.29	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	93	403157	10.0	6.05	
72 Ethyl methacrylate	69	6.868	6.868	0.000	89	358929	10.0	5.64	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	354459	10.0	8.29	
74 Tetrachloroethene	164	7.117	7.117	0.000	95	485576	10.0	10.4	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	92	604392	10.0	8.04	
76 2-Hexanone	43	7.188	7.188	0.000	96	346746	20.0	10.6	
79 Chlorodibromomethane	129	7.342	7.342	0.000	89	335695	10.0	7.52	
80 Ethylene Dibromide	107	7.461	7.461	0.000	98	346752	10.0	7.58	
82 Chlorobenzene	112	7.900	7.900	0.000	96	1303935	10.0	9.30	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	92	442333	10.0	8.94	
84 Ethylbenzene	106	7.995	7.995	0.000	98	657109	10.0	8.91	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	1576886	10.0	9.01	
86 o-Xylene	106	8.481	8.481	0.000	96	823918	10.0	9.29	
87 Styrene	104	8.493	8.493	0.000	92	1352213	10.0	9.11	
88 Bromoform	173	8.682	8.682	0.000	98	181279	10.0	5.60	
89 Isopropylbenzene	105	8.836	8.836	0.000	95	1899975	10.0	9.06	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	403472	10.0	6.36	
92 Bromobenzene	156	9.145	9.145	0.000	86	633082	10.0	8.55	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	67	64554	10.0	7.11	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	87	146688	10.0	6.64	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	536107	10.0	8.22	
97 2-Chlorotoluene	126	9.323	9.323	0.000	97	511353	10.0	8.38	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	1609431	10.0	8.49	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	1623337	10.0	8.22	
101 tert-Butylbenzene	119	9.714	9.714	0.000	91	1356815	10.0	7.99	
103 1,2,4-Trimethylbenzene	105	9.761	9.761	0.000	94	1727148	10.0	8.66	
105 sec-Butylbenzene	105	9.927	9.927	0.000	93	1690257	10.0	8.12	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	97	1120354	10.0	8.79	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	96	1556241	10.0	8.35	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	97	1156649	10.0	8.75	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	1129871	10.0	7.66	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	99	1106878	10.0	8.92	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	91	60130	10.0	4.17	
115 1,2,4-Trichlorobenzene	180	12.109	12.109	0.000	93	614624	10.0	7.82	
116 Hexachlorobutadiene	225	12.275	12.275	0.000	91	309226	10.0	7.64	
117 Naphthalene	128	12.358	12.358	0.000	96	1113134	10.0	5.63	
118 1,2,3-Trichlorobenzene	180	12.607	12.607	0.000	95	570942	10.0	8.07	
S 129 Xylenes, Total	106				0		20.0	18.3	
S 157 Total BTEX	1		0.000				50.0	ND	
S 130 Trihalomethanes, Total	1				0		40.0	33.7	

Reagents:

VMRGAS_00283	Amount Added: 8.00	Units: uL	
VMRPRIMW_00324	Amount Added: 8.00	Units: uL	
VMAROLISTDW_00286	Amount Added: 8.00	Units: uL	
vm40ml_vials_00009	Amount Added: 0.00	Units:	Run Reagent
vm50ss_stk_00079	Amount Added: 0.80	Units: uL	Run Reagent
VM50IS_00072	Amount Added: 1.00	Units: uL	Run Reagent
vmDist_H2o_00139	Amount Added: 0.00	Units:	Run Reagent

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9085.D

Injection Date: 01-Mar-2019 11:33:30

Instrument ID: A3UX15

Operator ID:

Lims ID: CCVIS L4 8260

Worklist Smp#: 2

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 1

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

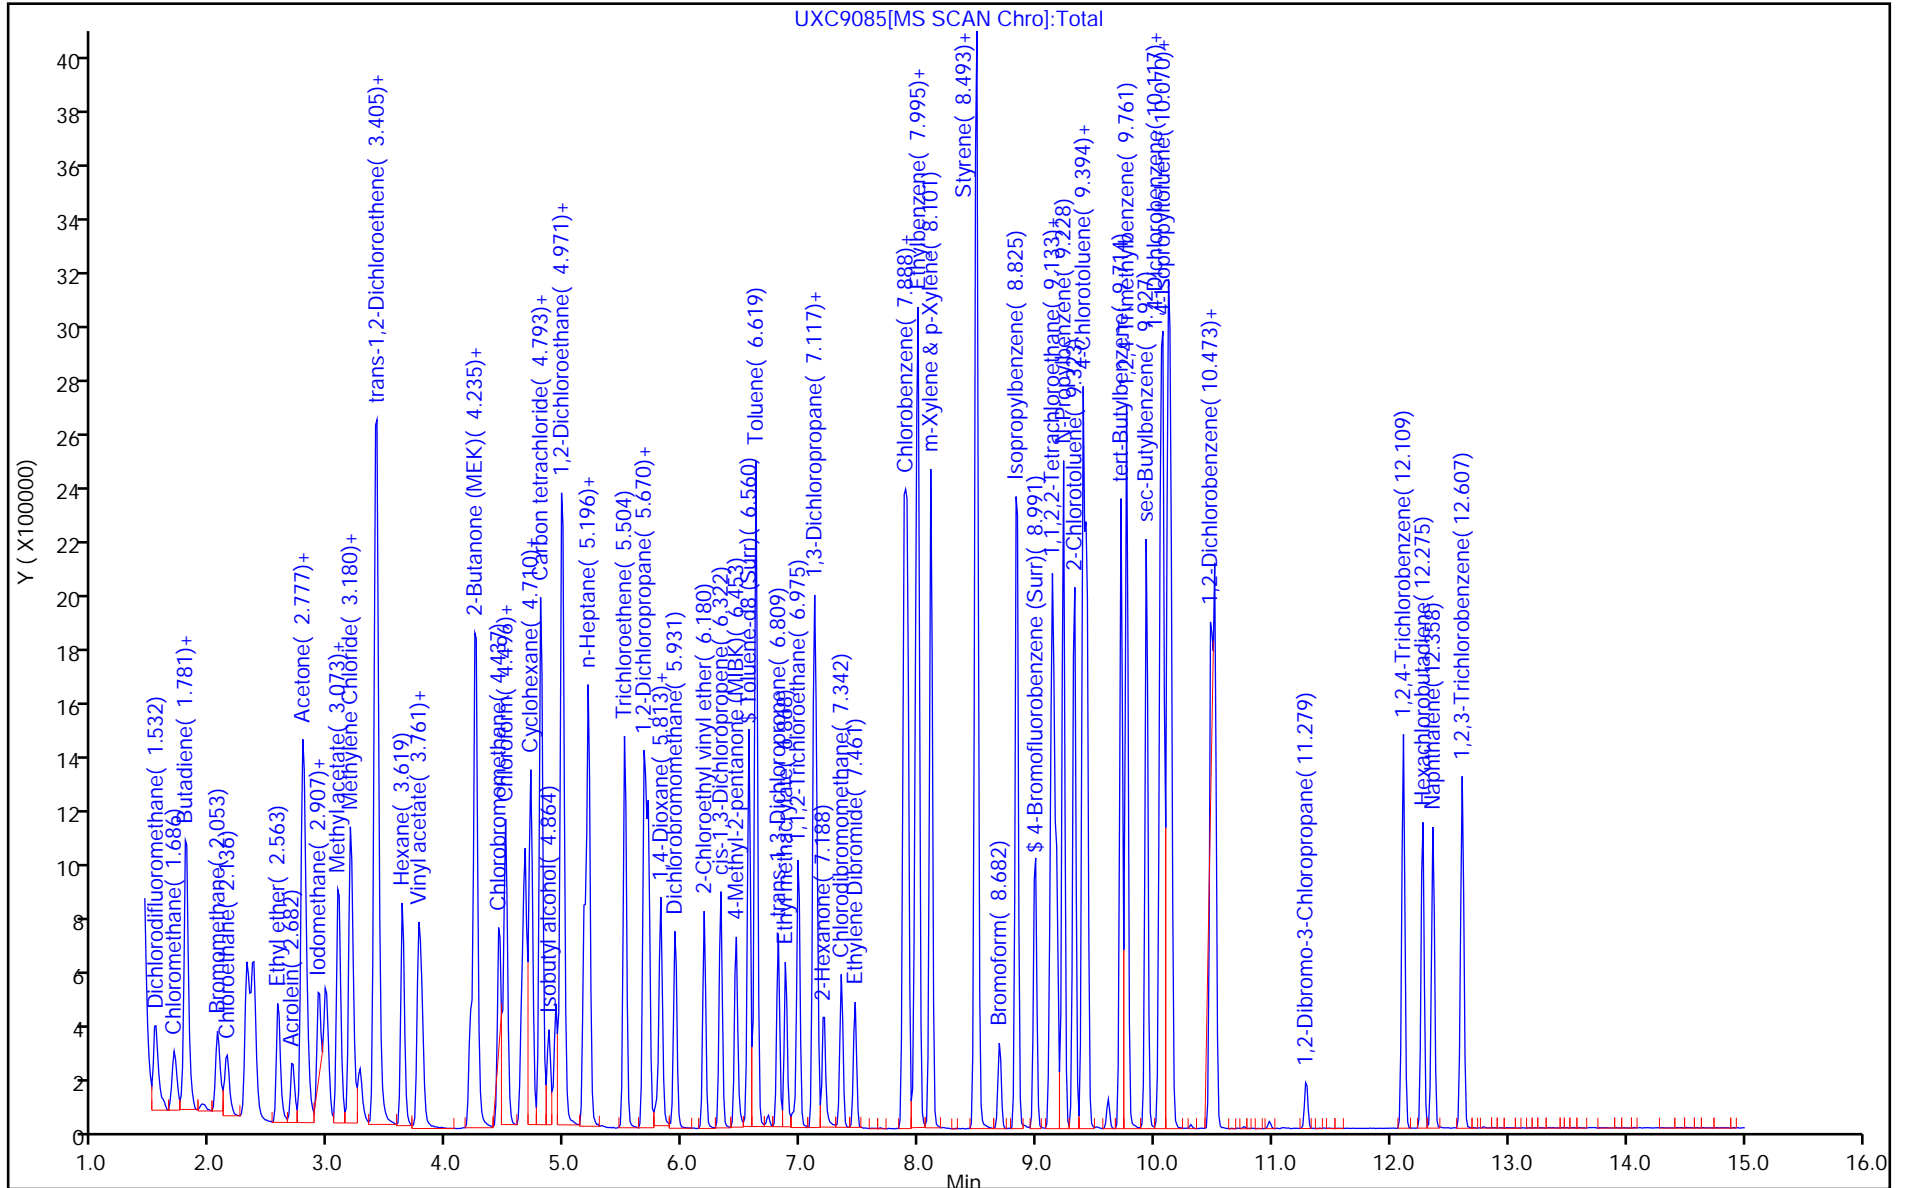

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	STD8260 240-364785/7	UXC8415.D
Level 2	STD8260 240-364785/6	UXC8414.D
Level 3	STD8260 240-364785/5	UXC8413.D
Level 4	STD8260 240-364785/4	UXC8412.D
Level 5	STD8260 240-364785/3	UXC8411.D
Level 6	STD8260 240-364785/2	UXC8410.D

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Dichlorodifluoromethane	0.2704 0.3071	0.3084	0.3222	0.3169	0.3182	Ave		0.3072			6.2		15.0				
Chloromethane	0.3289 0.2976	0.3274	0.3004	0.3124	0.3145	Ave		0.3135		0.1000	4.2		15.0				
Vinyl chloride	0.3261 0.2600	0.2864	0.2844	0.3065	0.2674	Ave		0.2885			8.5		15.0				
Butadiene	0.4028 0.3420	0.4066	0.3934	0.3729	0.3588	Ave		0.3794			6.8		15.0				
Bromomethane	0.2686 0.1933	0.2748	0.2163	0.2258	0.2060	Ave		0.2308			14.5		15.0				
Chloroethane	0.2298 0.1805	0.2264	0.1983	0.1989	0.1909	Ave		0.2041			9.7		15.0				
Dichlorofluoromethane	0.5874 0.4462	0.5508	0.5133	0.4857	0.4776	Ave		0.5102			10.1		15.0				
Trichlorofluoromethane	0.3885 0.4373	0.4314	0.4444	0.4568	0.4435	Ave		0.4337			5.5		15.0				
Ethyl ether	0.2527 0.2122	0.2393	0.2313	0.2239	0.2264	Ave		0.2310			6.0		15.0				
Acrolein	0.0365 0.0295	0.0303	0.0315	0.0310	0.0314	Ave		0.0317			7.8		15.0				
1,1-Dichloroethene	0.3235 0.2800	0.3292	0.3015	0.2758	0.2929	Ave		0.3005			7.3		15.0				
1,1,2-Trichloro-1,2,2-trifluoroethane	0.2411 0.2414	0.2509	0.2485	0.2467	0.2520	Ave		0.2468			1.9		15.0				
Acetone	0.0487 0.0213	0.0318	0.0276	0.0238	0.0247	Lin1	0.0519	0.0216						0.9960		0.9900	
Iodomethane	0.5303 0.4178	0.4271	0.4860	0.4853	0.4584	Ave		0.4675			9.0		15.0				
Carbon disulfide	0.9104 0.6640	0.7771	0.8074	0.7715	0.7145	Ave		0.7741			10.9		15.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
3-Chloro-1-propene	0.1530 0.1820	0.1600	0.1683	0.1693	0.1865	Ave		0.1698			7.5		15.0				
Methyl acetate	0.2259 0.1968	0.2056	0.2072	0.1929	0.2018	Ave		0.2050			5.6		15.0				
Methylene Chloride	0.8777 0.2608	0.5429	0.3681	0.3100	0.2858	Lin1	0.6169	0.2481						0.9990		0.9900	
2-Methyl-2-propanol	0.0205 0.0194	0.0225	0.0201	0.0175	0.0217	Ave		0.0203			8.7		15.0				
Acrylonitrile	0.0992 0.0981	0.0964	0.0945	0.0907	0.0981	Ave		0.0962			3.3		15.0				
Methyl tert-butyl ether	0.7930 0.7799	0.7813	0.7775	0.7682	0.8007	Ave		0.7834			1.5		15.0				
trans-1,2-Dichloroethene	0.3101 0.2660	0.2823	0.2736	0.2669	0.2784	Ave		0.2795			5.8		15.0				
Hexane	0.0608 0.0585	0.0607	0.0559	0.0560	0.0600	Ave		0.0586			3.8		15.0				
1,1-Dichloroethane	0.4596 0.4425	0.4568	0.4457	0.4441	0.4617	Ave		0.4517		0.1000	1.9		15.0				
Vinyl acetate	0.4987 0.5397	0.4861	0.5183	0.5294	0.5465	Ave		0.5198			4.5		15.0				
cis-1,2-Dichloroethene	0.3231 0.2906	0.3188	0.3032	0.3017	0.3096	Ave		0.3078			3.9		15.0				
2,2-Dichloropropane	0.0662 0.0571	0.0600	0.0637	0.0645	0.0628	Ave		0.0624			5.3		15.0				
2-Butanone (MEK)	0.0354 0.0328	0.0334	0.0325	0.0320	0.0334	Ave		0.0333			3.6		15.0				
Chlorobromomethane	0.1617 0.1477	0.1552	0.1523	0.1470	0.1549	Ave		0.1531			3.6		15.0				
Tetrahydrofuran	0.0906 0.0816	0.0853	0.0820	0.0745	0.0826	Ave		0.0828			6.4		15.0				
Chloroform	0.4755 0.4441	0.4649	0.4595	0.4523	0.4670	Ave		0.4606			2.4		15.0				
1,1,1-Trichloroethane	0.3615 0.3251	0.3567	0.3634	0.3678	0.3533	Ave		0.3546			4.3		15.0				
Cyclohexane	0.3905 0.3986	0.3949	0.4008	0.3961	0.4147	Ave		0.3993			2.1		15.0				
1,1-Dichloropropene	0.3764 0.3614	0.3858	0.3737	0.3673	0.3839	Ave		0.3748			2.5		15.0				
Carbon tetrachloride	0.3226 0.3473	0.3407	0.3468	0.3462	0.3607	Ave		0.3441			3.6		15.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Isobutyl alcohol	0.0072 0.0077	0.0080	0.0077	0.0069	0.0086	Ave		0.0077			7.7		15.0				
Benzene	1.1739 1.0767	1.1296	1.1053	1.0802	1.1333	Ave		1.1165			3.3		15.0				
1,2-Dichloroethane	0.3855 0.3692	0.3897	0.3815	0.3777	0.3886	Ave		0.3820			2.0		15.0				
n-Heptane	0.0499 0.0533	0.0523	0.0527	0.0543	0.0568	Ave		0.0532			4.3		15.0				
Trichloroethene	0.3350 0.3084	0.3298	0.3223	0.3165	0.3318	Ave		0.3240			3.1		15.0				
Methylcyclohexane	0.3407 0.3494	0.3484	0.3548	0.3494	0.3719	Ave		0.3524			3.0		15.0				
1,2-Dichloropropane	0.2476 0.2542	0.2676	0.2609	0.2580	0.2658	Ave		0.2590			2.9		15.0				
Dibromomethane	0.1763 0.1613	0.1789	0.1712	0.1695	0.1730	Ave		0.1717			3.6		15.0				
1,4-Dioxane	0.0015 0.0021	0.0019	0.0021	0.0019	0.0024	Lin1	-0.013	0.0022						0.9940		0.9900	
Dichlorobromomethane	0.3251 0.3470	0.3335	0.3329	0.3402	0.3670	Ave		0.3410			4.3		15.0				
2-Chloroethyl vinyl ether	0.1741 0.1794	0.1688	0.1738	0.1710	0.1802	Ave		0.1745			2.6		15.0				
cis-1,3-Dichloropropene	0.3518 0.4202	0.3782	0.3877	0.3983	0.4304	Ave		0.3944			7.3		15.0				
4-Methyl-2-pentanone (MIBK)	0.2785 0.2686	0.2562	0.2693	0.2591	0.2753	Ave		0.2678			3.3		15.0				
Toluene	1.5012 1.4288	1.4730	1.4635	1.4625	1.5286	Ave		1.4763			2.3		15.0				
trans-1,3-Dichloropropene	0.4131 0.5013	0.4307	0.4524	0.4755	0.5145	Ave		0.4646			8.6		15.0				
Ethyl methacrylate	0.4397 0.4538	0.4440	0.4290	0.4357	0.4632	Ave		0.4442			2.8		15.0				
1,1,2-Trichloroethane	0.2996 0.2912	0.3009	0.2966	0.2943	0.3064	Ave		0.2982			1.8		15.0				
Tetrachloroethene	0.3214 0.3151	0.3301	0.3272	0.3250	0.3419	Ave		0.3268			2.8		15.0				
1,3-Dichloropropane	0.5170 0.5210	0.5290	0.5125	0.5245	0.5419	Ave		0.5243			2.0		15.0				
2-Hexanone	0.2098 0.2323	0.2329	0.2285	0.2242	0.2423	Ave		0.2283			4.8		15.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Chlorodibromomethane	0.2647 0.3480	0.2850	0.3021	0.3162	0.3534	Ave		0.3116			11.2		15.0				
Ethylene Dibromide	0.3243 0.3131	0.3134	0.3221	0.3160	0.3258	Ave		0.3191			1.8		15.0				
Chlorobenzene	0.9888 0.9546	0.9840	0.9675	0.9702	1.0011	Ave		0.9777		0.3000	1.7		15.0				
1,1,1,2-Tetrachloroethane	0.3344 0.3512	0.3269	0.3433	0.3517	0.3627	Ave		0.3450			3.8		15.0				
Ethylbenzene	0.5276 0.5075	0.5044	0.5075	0.5104	0.5293	Ave		0.5145			2.1		15.0				
m-Xylene & p-Xylene	1.2031 1.2384	1.2096	1.1828	1.2237	1.2677	Ave		1.2209			2.4		15.0				
o-Xylene	0.6311 0.6050	0.6086	0.6092	0.6181	0.6414	Ave		0.6189			2.3		15.0				
Styrene	0.9861 1.0619	0.9946	1.0226	1.0439	1.1061	Ave		1.0359			4.3		15.0				
Bromoform	0.1422 0.2592	0.1774	0.1876	0.2065	0.2510	Lin1	-0.162	0.2546		0.1000				0.9940		0.9900	
Isopropylbenzene	1.4236 1.4623	1.4332	1.4499	1.4809	1.5299	Ave		1.4633			2.6		15.0				
1,1,2,2-Tetrachloroethane	0.7263 0.6975	0.7108	0.7013	0.6946	0.7209	Ave		0.7086		0.3000	1.8		15.0				
Bromobenzene	0.8425 0.8141	0.8308	0.8169	0.8158	0.8444	Ave		0.8274			1.7		15.0				
1,2,3-Trichloropropane	0.2495 0.2424	0.2553	0.2455	0.2417	0.2464	Ave		0.2468			2.0		15.0				
trans-1,4-Dichloro-2-butene	0.0434 0.1642	0.1010	0.0590	0.0798	0.1609	Ave		0.1014			50.5	*	15.0				
N-Propylbenzene	0.7265 0.7228	0.7398	0.7179	0.7231	0.7419	Ave		0.7286			1.3		15.0				
2-Chlorotoluene	0.7109 0.6635	0.6787	0.6802	0.6673	0.6918	Ave		0.6821			2.5		15.0				
1,3,5-Trimethylbenzene	2.1272 2.0859	2.0953	2.0772	2.1235	2.2036	Ave		2.1188			2.2		15.0				
4-Chlorotoluene	2.2568 2.1504	2.2467	2.1776	2.1619	2.2388	Ave		2.2054			2.1		15.0				
tert-Butylbenzene	1.8677 1.9925	1.8939	1.8513	1.8658	1.9133	Ave		1.8974			2.7		15.0				
1,2,4-Trimethylbenzene	2.2391 2.1885	2.2675	2.1657	2.2226	2.2813	Ave		2.2275			2.0		15.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
sec-Butylbenzene	2.2915 2.2504	2.3538	2.3171	2.3275	2.4198	Ave		2.3267			2.5		15.0				
1,3-Dichlorobenzene	1.4983 1.3538	1.4434	1.4148	1.4043	1.4340	Ave		1.4248			3.4		15.0				
4-Isopropyltoluene	2.0430 2.0131	2.1052	2.0529	2.1055	2.1774	Ave		2.0829			2.8		15.0				
1,4-Dichlorobenzene	1.5786 1.4104	1.5222	1.4387	1.4418	1.4716	Ave		1.4772			4.2		15.0				
n-Butylbenzene	1.6870 1.5530	1.6578	1.6297	1.6645	1.6997	Ave		1.6486			3.2		15.0				
1,2-Dichlorobenzene	1.4437 1.3061	1.4168	1.3751	1.3937	1.3869	Ave		1.3871			3.4		15.0				
1,2-Dibromo-3-Chloropropane	0.1400 0.1672	0.1533	0.1616	0.1661	0.1785	Ave		0.1611			8.2		15.0				
1,2,4-Trichlorobenzene	0.9724 0.7297	0.9185	0.8808	0.8895	0.8794	Ave		0.8784			9.2		15.0				
Hexachlorobutadiene	0.5543 0.3117	0.4931	0.4340	0.4326	0.4056	Qua	-0.024	0.4891	-0.004405					0.9990		0.9900	
Naphthalene	2.2857 1.9486	2.1983	2.2894	2.2740	2.2589	Ave		2.2091			6.0		15.0				
1,2,3-Trichlorobenzene	0.8662 0.6533	0.8274	0.8022	0.7980	0.7943	Ave		0.7902			9.1		15.0				
Dibromofluoromethane (Surr)	0.2371 0.2318	0.2202	0.2449	0.2390	0.2468	Ave		0.2366			4.1		15.0				
1,2-Dichloroethane-d4 (Surr)	0.3138 0.2896	0.2914	0.3140	0.3062	0.3101	Ave		0.3042			3.6		15.0				
Toluene-d8 (Surr)	1.2471 1.1640	1.1461	1.2369	1.2229	1.2656	Ave		1.2138			3.9		15.0				
4-Bromofluorobenzene (Surr)	0.4328 0.4271	0.4150	0.4450	0.4370	0.4478	Ave		0.4341			2.8		15.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	STD8260 240-364785/7	UXC8415.D
Level 2	STD8260 240-364785/6	UXC8414.D
Level 3	STD8260 240-364785/5	UXC8413.D
Level 4	STD8260 240-364785/4	UXC8412.D
Level 5	STD8260 240-364785/3	UXC8411.D
Level 6	STD8260 240-364785/2	UXC8410.D

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (UG/L)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Dichlorodifluoromethane	FB	Ave	47729 2392918	112693	296202	593761	1222220	1.00 40.0	2.00	5.00	10.0	20.0
Chloromethane	FB	Ave	58046 2319242	119628	276149	585358	1207742	1.00 40.0	2.00	5.00	10.0	20.0
Vinyl chloride	FB	Ave	57558 2025909	104647	261470	574312	1027051	1.00 40.0	2.00	5.00	10.0	20.0
Butadiene	FB	Ave	71088 2665435	148568	361713	698736	1378009	1.00 40.0	2.00	5.00	10.0	20.0
Bromomethane	FB	Ave	47411 1506749	100403	198900	423055	791041	1.00 40.0	2.00	5.00	10.0	20.0
Chloroethane	FB	Ave	40558 1406432	82718	182320	372694	733356	1.00 40.0	2.00	5.00	10.0	20.0
Dichlorofluoromethane	FB	Ave	103682 3477509	201291	471934	910063	1834172	1.00 40.0	2.00	5.00	10.0	20.0
Trichlorofluoromethane	FB	Ave	68568 3407867	157640	408598	855986	1703371	1.00 40.0	2.00	5.00	10.0	20.0
Ethyl ether	FB	Ave	44605 1653914	87432	212667	419544	869536	1.00 40.0	2.00	5.00	10.0	20.0
Acrolein	FB	Ave	32229 1148055	55282	144856	290454	603583	5.00 200	10.0	25.0	50.0	100
1,1-Dichloroethene	FB	Ave	57094 2182381	120279	277159	516876	1125076	1.00 40.0	2.00	5.00	10.0	20.0
1,1,2-Trichloro-1,2,2-trifluoroethane	FB	Ave	42550 1880984	91700	228498	462285	967763	1.00 40.0	2.00	5.00	10.0	20.0
Acetone	FB	Lin1	17181 332724	23252	50751	89168	190030	2.00 80.0	4.00	10.0	20.0	40.0
Iodomethane	FB	Ave	93588 3255913	156089	446819	909454	1760595	1.00 40.0	2.00	5.00	10.0	20.0
Carbon disulfide	FB	Ave	160687 5174431	283969	742305	1445567	2744114	1.00 40.0	2.00	5.00	10.0	20.0
3-Chloro-1-propene	FB	Ave	27003 1418141	58477	154763	317161	716236	1.00 40.0	2.00	5.00	10.0	20.0

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (UG/L)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Methyl acetate	FB	Ave	79740 3067156	150240	380996	723073	1550490	2.00 80.0	4.00	10.0	20.0	40.0
Methylene Chloride	FB	Lin1	154915 2032773	198393	338417	580808	1097865	1.00 40.0	2.00	5.00	10.0	20.0
2-Methyl-2-propanol	FB	Ave	36240 1508945	82343	184510	328142	832907	10.0 400	20.0	50.0	100	200
Acrylonitrile	FB	Ave	175156 7643188	352291	868795	1699336	3768272	10.0 400	20.0	50.0	100	200
Methyl tert-butyl ether	FB	Ave	139955 6078083	285516	714788	1439491	3075308	1.00 40.0	2.00	5.00	10.0	20.0
trans-1,2-Dichloroethene	FB	Ave	54736 2072831	103155	251570	500088	1069131	1.00 40.0	2.00	5.00	10.0	20.0
Hexane	FB	Ave	10725 455555	22194	51427	104918	230317	1.00 40.0	2.00	5.00	10.0	20.0
1,1-Dichloroethane	FB	Ave	81126 3448011	166930	409730	832192	1773410	1.00 40.0	2.00	5.00	10.0	20.0
Vinyl acetate	FB	Ave	88027 4206187	177639	476538	992089	2098831	1.00 40.0	2.00	5.00	10.0	20.0
cis-1,2-Dichloroethene	FB	Ave	57035 2264494	116480	278759	565374	1189038	1.00 40.0	2.00	5.00	10.0	20.0
2,2-Dichloropropane	FB	Ave	11684 445323	21907	58586	120845	241048	1.00 40.0	2.00	5.00	10.0	20.0
2-Butanone (MEK)	FB	Ave	12505 511818	24387	59681	120010	256717	2.00 80.0	4.00	10.0	20.0	40.0
Chlorobromomethane	FB	Ave	28543 1150919	56716	140018	275468	595090	1.00 40.0	2.00	5.00	10.0	20.0
Tetrahydrofuran	FB	Ave	31985 1272086	62314	150812	279158	634219	2.00 80.0	4.00	10.0	20.0	40.0
Chloroform	FB	Ave	83929 3460990	169874	422474	847597	1793716	1.00 40.0	2.00	5.00	10.0	20.0
1,1,1-Trichloroethane	FB	Ave	63803 2533663	130349	334136	689229	1356966	1.00 40.0	2.00	5.00	10.0	20.0
Cyclohexane	FB	Ave	68915 3105972	144320	368473	742256	1592895	1.00 40.0	2.00	5.00	10.0	20.0
1,1-Dichloropropene	FB	Ave	66437 2816568	140972	343617	688186	1474449	1.00 40.0	2.00	5.00	10.0	20.0
Carbon tetrachloride	FB	Ave	56945 2706723	124489	318843	648774	1385341	1.00 40.0	2.00	5.00	10.0	20.0
Isobutyl alcohol	FB	Ave	31904 1496664	73133	177736	322275	821992	25.0 1000	50.0	125	250	500
Benzene	FB	Ave	207184 8390558	412777	1016161	2024145	4352726	1.00 40.0	2.00	5.00	10.0	20.0

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (UG/L)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
1,2-Dichloroethane	FB	Ave	68031 2877185	142414	350758	707702	1492475	1.00 40.0	2.00	5.00	10.0	20.0
n-Heptane	FB	Ave	8801 415529	19095	48491	101813	218160	1.00 40.0	2.00	5.00	10.0	20.0
Trichloroethene	FB	Ave	59121 2403531	120531	296310	593061	1274454	1.00 40.0	2.00	5.00	10.0	20.0
Methylcyclohexane	FB	Ave	60130 2723193	127322	326169	654672	1428283	1.00 40.0	2.00	5.00	10.0	20.0
1,2-Dichloropropane	FB	Ave	43707 1981074	97800	239856	483376	1020861	1.00 40.0	2.00	5.00	10.0	20.0
Dibromomethane	FB	Ave	31111 1256838	65366	157375	317664	664429	1.00 40.0	2.00	5.00	10.0	20.0
1,4-Dioxane	FB	Lin1	5185 326819	14227	39232	71764	183906	20.0 800	40.0	100	200	400
Dichlorobromomethane	FB	Ave	57382 2704273	121869	306036	637533	1409597	1.00 40.0	2.00	5.00	10.0	20.0
2-Chloroethyl vinyl ether	FB	Ave	61442 2796269	123378	319533	640886	1383920	2.00 80.0	4.00	10.0	20.0	40.0
cis-1,3-Dichloropropene	FB	Ave	62099 3274371	138202	356486	746312	1652896	1.00 40.0	2.00	5.00	10.0	20.0
4-Methyl-2-pentanone (MIBK)	FB	Ave	98299 4186633	187250	495239	970866	2114735	2.00 80.0	4.00	10.0	20.0	40.0
Toluene	CBNZ d5	Ave	209687 9034071	428381	1080197	2172974	4691174	1.00 40.0	2.00	5.00	10.0	20.0
trans-1,3-Dichloropropene	CBNZ d5	Ave	57707 3169409	125256	333930	706531	1578892	1.00 40.0	2.00	5.00	10.0	20.0
Ethyl methacrylate	CBNZ d5	Ave	61421 2869285	129112	316654	647349	1421429	1.00 40.0	2.00	5.00	10.0	20.0
1,1,2-Trichloroethane	CBNZ d5	Ave	41853 1840913	87521	218933	437245	940456	1.00 40.0	2.00	5.00	10.0	20.0
Tetrachloroethene	CBNZ d5	Ave	44889 1992562	95990	241473	482895	1049416	1.00 40.0	2.00	5.00	10.0	20.0
1,3-Dichloropropane	CBNZ d5	Ave	72217 3294456	153833	378264	779324	1663194	1.00 40.0	2.00	5.00	10.0	20.0
2-Hexanone	CBNZ d5	Ave	58616 2937075	135481	337296	666112	1487023	2.00 80.0	4.00	10.0	20.0	40.0
Chlorodibromomethane	CBNZ d5	Ave	36977 2200067	82891	222991	469828	1084488	1.00 40.0	2.00	5.00	10.0	20.0
Ethylene Dibromide	CBNZ d5	Ave	45295 1979685	91132	237763	469490	999728	1.00 40.0	2.00	5.00	10.0	20.0
Chlorobenzene	CBNZ d5	Ave	138107 6035718	286159	714138	1441533	3072375	1.00 40.0	2.00	5.00	10.0	20.0

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (UG/L)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
1,1,1,2-Tetrachloroethane	CBNZ d5	Ave	46702 2220799	95060	253355	522591	1113186	1.00 40.0	2.00	5.00	10.0	20.0
Ethylbenzene	CBNZ d5	Ave	73699 3208633	146696	374569	758362	1624425	1.00 40.0	2.00	5.00	10.0	20.0
m-Xylene & p-Xylene	CBNZ d5	Ave	168049 7830315	351787	872988	1818169	3890600	1.00 40.0	2.00	5.00	10.0	20.0
o-Xylene	CBNZ d5	Ave	88147 3825283	176986	449671	918350	1968397	1.00 40.0	2.00	5.00	10.0	20.0
Styrene	CBNZ d5	Ave	137740 6714209	289260	754758	1550959	3394736	1.00 40.0	2.00	5.00	10.0	20.0
Bromoform	CBNZ d5	Lin1	19867 1639155	51580	138461	306750	770158	1.00 40.0	2.00	5.00	10.0	20.0
Isopropylbenzene	CBNZ d5	Ave	198841 9246149	416807	1070139	2200366	4695119	1.00 40.0	2.00	5.00	10.0	20.0
1,1,2,2-Tetrachloroethane	DCBd 4	Ave	54865 2441270	112833	283791	577712	1238040	1.00 40.0	2.00	5.00	10.0	20.0
Bromobenzene	DCBd 4	Ave	63640 2849353	131876	330598	678570	1450127	1.00 40.0	2.00	5.00	10.0	20.0
1,2,3-Trichloropropane	DCBd 4	Ave	18846 848462	40526	99350	201010	423192	1.00 40.0	2.00	5.00	10.0	20.0
trans-1,4-Dichloro-2-butene	DCBd 4	Ave	3277 574750	16039	23872	66363	276245	1.00 40.0	2.00	5.00	10.0	20.0
N-Propylbenzene	DCBd 4	Ave	54874 2529942	117423	290505	601438	1274023	1.00 40.0	2.00	5.00	10.0	20.0
2-Chlorotoluene	DCBd 4	Ave	53702 2322347	107735	275264	555062	1188057	1.00 40.0	2.00	5.00	10.0	20.0
1,3,5-Trimethylbenzene	DCBd 4	Ave	160683 7300680	332591	840604	1766210	3784392	1.00 40.0	2.00	5.00	10.0	20.0
4-Chlorotoluene	DCBd 4	Ave	170473 7526400	356628	881245	1798133	3844885	1.00 40.0	2.00	5.00	10.0	20.0
tert-Butylbenzene	DCBd 4	Ave	141080 6973779	300630	749194	1551899	3285832	1.00 40.0	2.00	5.00	10.0	20.0
1,2,4-Trimethylbenzene	DCBd 4	Ave	169136 7660047	359918	876431	1848645	3917785	1.00 40.0	2.00	5.00	10.0	20.0
sec-Butylbenzene	DCBd 4	Ave	173094 7876504	373619	937713	1935865	4155710	1.00 40.0	2.00	5.00	10.0	20.0
1,3-Dichlorobenzene	DCBd 4	Ave	113176 4738373	229119	572540	1168047	2462678	1.00 40.0	2.00	5.00	10.0	20.0
4-Isopropyltoluene	DCBd 4	Ave	154318 7046098	334169	830781	1751242	3739399	1.00 40.0	2.00	5.00	10.0	20.0
1,4-Dichlorobenzene	DCBd 4	Ave	119243 4936571	241629	582208	1199185	2527274	1.00 40.0	2.00	5.00	10.0	20.0

FORM VI
GC/MS VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Canton Job No.: 240-108701-1 Analy Batch No.: 364785

SDG No.: _____

Instrument ID: A3UX15 GC Column: DB-624 ID: 0.18 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 01/21/2019 11:37 Calibration End Date: 01/21/2019 13:26 Calibration ID: 49063

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (UG/L)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
n-Butylbenzene	DCBd 4	Ave	127428 5435677	263153	659506	1384405	2918965	1.00 40.0	2.00	5.00	10.0	20.0
1,2-Dichlorobenzene	DCBd 4	Ave	109056 4571601	224899	556492	1159176	2381785	1.00 40.0	2.00	5.00	10.0	20.0
1,2-Dibromo-3-Chloropropane	DCBd 4	Ave	10572 585195	24334	65389	138143	306515	1.00 40.0	2.00	5.00	10.0	20.0
1,2,4-Trichlorobenzene	DCBd 4	Ave	73453 2553990	145803	356465	739836	1510157	1.00 40.0	2.00	5.00	10.0	20.0
Hexachlorobutadiene	DCBd 4	Qua	41867 1091039	78276	175613	359850	696597	1.00 40.0	2.00	5.00	10.0	20.0
Naphthalene	DCBd 4	Ave	172653 6820199	348942	926474	1891386	3879317	1.00 40.0	2.00	5.00	10.0	20.0
1,2,3-Trichlorobenzene	DCBd 4	Ave	65430 2286670	131338	324635	663704	1364016	1.00 40.0	2.00	5.00	10.0	20.0
Dibromofluoromethane (Surr)	FB	Ave	41840 1806247	80448	225163	447792	947952	1.00 40.0	2.00	5.00	10.0	20.0
1,2-Dichloroethane-d4 (Surr)	FB	Ave	55383 2257190	106482	288691	573781	1190875	1.00 40.0	2.00	5.00	10.0	20.0
Toluene-d8 (Surr)	CBNZ d5	Ave	174193 7359833	333303	912990	1816996	3883966	1.00 40.0	2.00	5.00	10.0	20.0
4-Bromofluorobenzene (Surr)	CBNZ d5	Ave	60446 2700470	120695	328418	649263	1374232	1.00 40.0	2.00	5.00	10.0	20.0

Curve Type Legend:

Ave = Average ISTD
Linl = Linear 1/conc ISTD
Qua = Quadratic ISTD

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8410.D
 Lims ID: STD8260 L6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 21-Jan-2019 11:37:30 ALS Bottle#: 1 Worklist Smp#: 2
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-002
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:12:44 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

First Level Reviewer: evansle

Date: 22-Jan-2019 09:12:32

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.208	5.196	0.012	99	1948244	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1580707	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	91	875018	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	1806247	40.0	39.2	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	2257190	40.0	38.1	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	7359833	40.0	38.4	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	97	2700470	40.0	39.4	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	2392918	40.0	40.0	
10 Chloromethane	50	1.698	1.686	0.012	99	2319242	40.0	38.0	
11 Vinyl chloride	62	1.793	1.781	0.012	98	2025909	40.0	36.0	
12 Butadiene	54	1.804	1.793	0.011	98	2665435	40.0	36.1	
13 Bromomethane	94	2.065	2.054	0.011	90	1506749	40.0	33.5	
14 Chloroethane	64	2.160	2.137	0.023	100	1406432	40.0	35.4	
15 Dichlorofluoromethane	67	2.314	2.303	0.011	97	3477509	40.0	35.0	
16 Trichlorofluoromethane	101	2.362	2.362	0.000	98	3407867	40.0	40.3	
17 Ethyl ether	59	2.575	2.563	0.012	89	1653914	40.0	36.8	
18 Acrolein	56	2.694	2.694	0.000	100	1148055	200.0	185.9	
19 1,1-Dichloroethene	96	2.812	2.777	0.035	98	2182381	40.0	37.3	
20 1,1,2-Trichloro-1,2,2-trif	151	2.812	2.789	0.023	79	1880984	40.0	39.1	
22 Acetone	58	2.824	2.812	0.012	99	332724	80.0	76.8	
23 Iodomethane	142	2.955	2.931	0.024	98	3255913	40.0	35.7	
24 Carbon disulfide	76	3.002	2.990	0.012	100	5174431	40.0	34.3	
25 3-Chloro-1-propene	76	3.085	3.073	0.012	88	1418141	40.0	42.9	
27 Methyl acetate	43	3.097	3.085	0.012	98	3067156	80.0	76.8	
28 Methylene Chloride	84	3.192	3.180	0.012	92	2032773	40.0	39.6	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	1508945	400.0	381.9	
32 Acrylonitrile	53	3.393	3.394	-0.001	99	7643188	400.0	407.9	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	6078083	40.0	39.8	
30 trans-1,2-Dichloroethene	96	3.417	3.405	0.012	95	2072831	40.0	38.1	
33 Hexane	86	3.631	3.619	0.012	93	455555	40.0	39.9	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	3448011	40.0	39.2	
36 Vinyl acetate	43	3.797	3.785	0.012	97	4206187	40.0	41.5	
39 cis-1,2-Dichloroethene	96	4.247	4.235	0.012	81	2264494	40.0	37.8	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	60	445323	40.0	36.6	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	99	511818	80.0	79.0	
45 Chlorobromomethane	128	4.449	4.449	0.000	89	1150919	40.0	38.6	
46 Tetrahydrofuran	42	4.484	4.485	-0.001	87	1272086	80.0	78.9	
47 Chloroform	83	4.508	4.496	0.012	93	3460990	40.0	38.6	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	98	2533663	40.0	36.7	
49 Cyclohexane	56	4.722	4.710	0.012	90	3105972	40.0	39.9	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	95	2816568	40.0	38.6	
50 Carbon tetrachloride	117	4.805	4.805	0.000	97	2706723	40.0	40.4	
52 Isobutyl alcohol	41	4.864	4.864	0.000	95	1496664	1000.0	1000.0	
53 Benzene	78	4.982	4.971	0.011	96	8390558	40.0	38.6	
54 1,2-Dichloroethane	62	4.994	4.983	0.011	98	2877185	40.0	38.7	
56 n-Heptane	100	5.172	5.160	0.012	93	415529	40.0	40.1	
58 Trichloroethene	130	5.516	5.504	0.012	96	2403531	40.0	38.1	
60 Methylcyclohexane	83	5.682	5.670	0.012	88	2723193	40.0	39.7	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	95	1981074	40.0	39.3	
64 1,4-Dioxane	88	5.813	5.813	0.000	59	326819	800.0	772.3	
63 Dibromomethane	93	5.813	5.813	0.000	88	1256838	40.0	37.6	
65 Dichlorobromomethane	83	5.931	5.931	0.000	99	2704273	40.0	40.7	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	2796269	80.0	82.2	
68 cis-1,3-Dichloropropene	75	6.322	6.323	-0.001	95	3274371	40.0	42.6	
69 4-Methyl-2-pentanone (MIBK)	43	6.453	6.441	0.012	97	4186633	80.0	80.2	
70 Toluene	91	6.619	6.619	0.000	98	9034071	40.0	38.7	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	94	3169409	40.0	43.2	
72 Ethyl methacrylate	69	6.868	6.868	0.000	89	2869285	40.0	40.9	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	1840913	40.0	39.1	
74 Tetrachloroethene	164	7.117	7.117	0.000	96	1992562	40.0	38.6	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	93	3294456	40.0	39.7	
76 2-Hexanone	43	7.188	7.188	0.000	97	2937075	80.0	81.4	
79 Chlorodibromomethane	129	7.342	7.342	0.000	90	2200067	40.0	44.7	
80 Ethylene Dibromide	107	7.461	7.461	0.000	98	1979685	40.0	39.2	
82 Chlorobenzene	112	7.900	7.900	0.000	96	6035718	40.0	39.1	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	94	2220799	40.0	40.7	
84 Ethylbenzene	106	7.995	7.995	0.000	98	3208633	40.0	39.5	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	7830315	40.0	40.6	
86 o-Xylene	106	8.481	8.481	0.000	97	3825283	40.0	39.1	
87 Styrene	104	8.493	8.493	0.000	94	6714209	40.0	41.0	
88 Bromoform	173	8.682	8.682	0.000	98	1639155	40.0	41.4	
89 Isopropylbenzene	105	8.825	8.825	0.000	95	9246149	40.0	40.0	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	2441270	40.0	39.4	
92 Bromobenzene	156	9.145	9.133	0.012	90	2849353	40.0	39.4	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	85	848462	40.0	39.3	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	80	574750	40.0	64.8	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	2529942	40.0	39.7	
97 2-Chlorotoluene	126	9.323	9.323	0.000	98	2322347	40.0	38.9	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	7300680	40.0	39.4	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	7526400	40.0	39.0	
101 tert-Butylbenzene	119	9.714	9.714	0.000	92	6973779	40.0	42.0	
103 1,2,4-Trimethylbenzene	105	9.761	9.762	-0.001	94	7660047	40.0	39.3	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
105 sec-Butylbenzene	105	9.927	9.928	-0.001	93	7876504	40.0	38.7	
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	98	4738373	40.0	38.0	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	97	7046098	40.0	38.7	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	97	4936571	40.0	38.2	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	5435677	40.0	37.7	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	99	4571601	40.0	37.7	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	93	585195	40.0	41.5	
115 1,2,4-Trichlorobenzene	180	12.109	12.110	-0.001	94	2553990	40.0	33.2	
116 Hexachlorobutadiene	225	12.275	12.276	-0.001	93	1091039	40.0	39.8	
117 Naphthalene	128	12.358	12.359	-0.001	96	6820199	40.0	35.3	
118 1,2,3-Trichlorobenzene	180	12.608	12.608	0.000	95	2286670	40.0	33.1	
S 127 1,2-Dichloroethene, Total	96				0			75.8	
S 128 1,3-Dichloropropene, Total	75				0			85.8	
S 129 Xylenes, Total	106				0		80.0	79.7	
S 130 Trihalomethanes, Total	1				0		160.0	165.3	
S 157 Total BTEX	1		0.000				200.0	ND	

Reagents:

vm50ss_stk_00079	Amount Added: 32.00	Units: uL
VM50IS_00072	Amount Added: 1.00	Units: uL
VMRPRIMW_00318	Amount Added: 32.00	Units: uL
VMAROLISTDW_00281	Amount Added: 32.00	Units: uL
VMRGAS_00278	Amount Added: 32.00	Units: uL

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8410.D

Injection Date: 21-Jan-2019 11:37:30

Instrument ID: A3UX15

Operator ID:

Lims ID: STD8260 L6

Worklist Smp#: 2

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 1

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

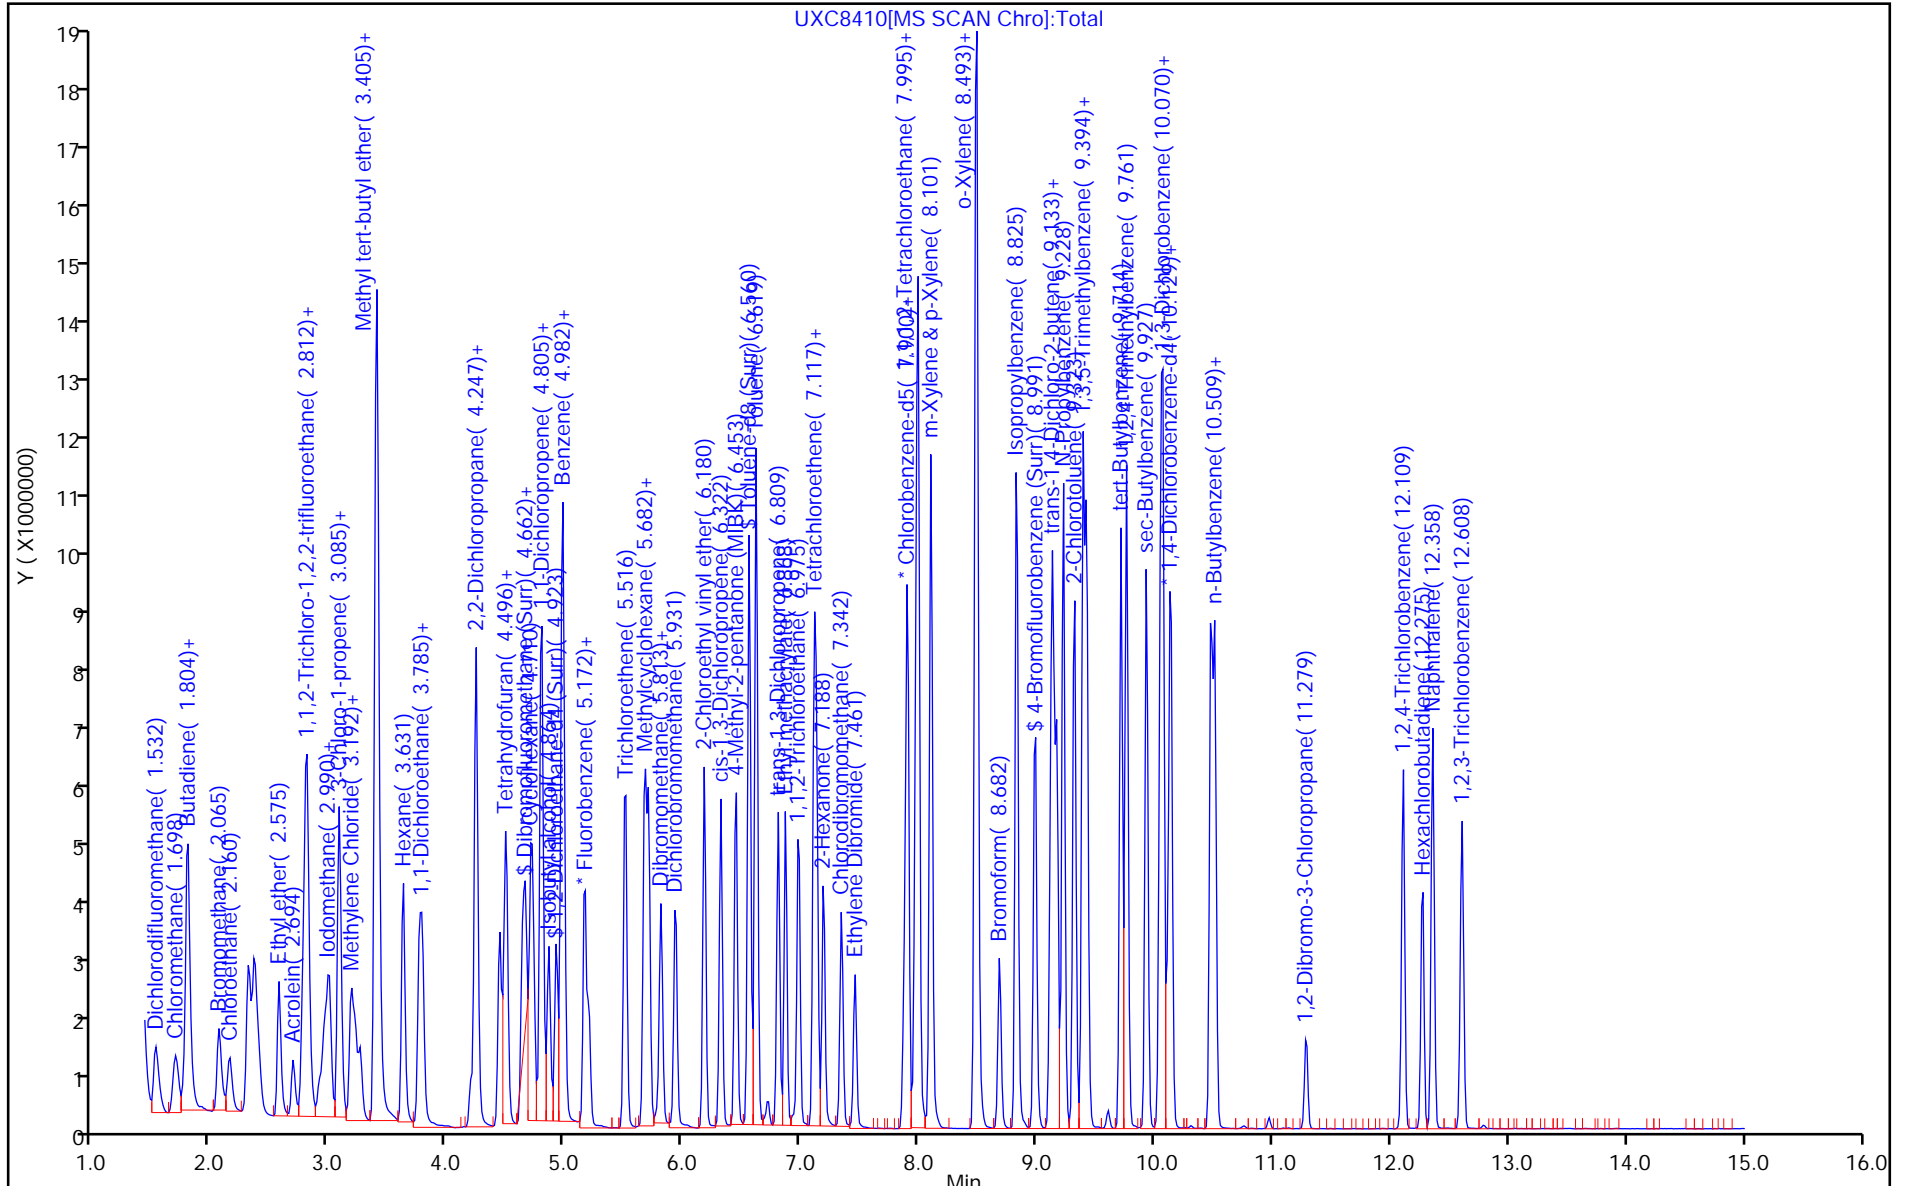

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8411.D
 Lims ID: STD8260 L5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 21-Jan-2019 11:59:30 ALS Bottle#: 2 Worklist Smp#: 3
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-003
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:09:37 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

First Level Reviewer: evansle

Date: 21-Jan-2019 12:41:50

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1920375	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1534484	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	90	858675	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	947952	20.0	20.9	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	1190875	20.0	20.4	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	3883966	20.0	20.9	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	96	1374232	20.0	20.6	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	1222220	20.0	20.7	
10 Chloromethane	50	1.698	1.686	0.012	99	1207742	20.0	20.1	
11 Vinyl chloride	62	1.793	1.781	0.012	98	1027051	20.0	18.5	
12 Butadiene	54	1.793	1.793	0.000	98	1378009	20.0	18.9	
13 Bromomethane	94	2.065	2.054	0.011	90	791041	20.0	17.8	
14 Chloroethane	64	2.160	2.137	0.023	100	733356	20.0	18.7	
15 Dichlorofluoromethane	67	2.314	2.303	0.011	98	1834172	20.0	18.7	
16 Trichlorofluoromethane	101	2.362	2.362	0.000	99	1703371	20.0	20.5	
17 Ethyl ether	59	2.575	2.563	0.012	90	869536	20.0	19.6	
18 Acrolein	56	2.694	2.694	0.000	99	603583	100.0	99.2	
19 1,1-Dichloroethene	96	2.801	2.777	0.024	98	1125076	20.0	19.5	
20 1,1,2-Trichloro-1,2,2-trif	151	2.801	2.789	0.012	78	967763	20.0	20.4	
22 Acetone	58	2.824	2.812	0.012	100	190030	40.0	43.5	
23 Iodomethane	142	2.955	2.931	0.024	98	1760595	20.0	19.6	
24 Carbon disulfide	76	3.002	2.990	0.012	100	2744114	20.0	18.5	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	88	716236	20.0	22.0	
27 Methyl acetate	43	3.085	3.085	0.000	98	1550490	40.0	39.4	
28 Methylene Chloride	84	3.180	3.180	0.000	92	1097865	20.0	20.6	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	832907	200.0	213.8	
32 Acrylonitrile	53	3.394	3.394	0.000	98	3768272	200.0	204.0	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	3075308	20.0	20.4	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	95	1069131	20.0	19.9	
33 Hexane	86	3.631	3.619	0.012	94	230317	20.0	20.5	

Compound	Sig	RT (min.)	Exp RT (min.)	Diff RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	1773410	20.0	20.4	
36 Vinyl acetate	43	3.785	3.785	0.000	97	2098831	20.0	21.0	
39 cis-1,2-Dichloroethene	96	4.247	4.235	0.012	81	1189038	20.0	20.1	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	65	241048	20.0	20.1	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	99	256717	40.0	40.2	
45 Chlorobromomethane	128	4.449	4.449	0.000	87	595090	20.0	20.2	
46 Tetrahydrofuran	42	4.485	4.485	0.000	87	634219	40.0	39.9	
47 Chloroform	83	4.496	4.496	0.000	93	1793716	20.0	20.3	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	98	1356966	20.0	19.9	
49 Cyclohexane	56	4.710	4.710	0.000	90	1592895	20.0	20.8	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	94	1474449	20.0	20.5	
50 Carbon tetrachloride	117	4.805	4.805	0.000	96	1385341	20.0	21.0	
52 Isobutyl alcohol	41	4.864	4.864	0.000	94	821992	500.0	557.2	
53 Benzene	78	4.971	4.971	0.000	95	4352726	20.0	20.3	
54 1,2-Dichloroethane	62	4.983	4.983	0.000	97	1492475	20.0	20.3	
56 n-Heptane	100	5.160	5.160	0.000	92	218160	20.0	21.3	
58 Trichloroethene	130	5.504	5.504	0.000	96	1274454	20.0	20.5	
60 Methylcyclohexane	83	5.670	5.670	0.000	90	1428283	20.0	21.1	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	95	1020861	20.0	20.5	
64 1,4-Dioxane	88	5.813	5.813	0.000	37	183906	400.0	443.3	
63 Dibromomethane	93	5.813	5.813	0.000	88	664429	20.0	20.2	
65 Dichlorobromomethane	83	5.931	5.931	0.000	99	1409597	20.0	21.5	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	1383920	40.0	41.3	
68 cis-1,3-Dichloropropene	75	6.323	6.323	0.000	94	1652896	20.0	21.8	
69 4-Methyl-2-pentanone (MIBK)	43	6.453	6.441	0.012	97	2114735	40.0	41.1	
70 Toluene	91	6.619	6.619	0.000	98	4691174	20.0	20.7	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	94	1578892	20.0	22.1	
72 Ethyl methacrylate	69	6.868	6.868	0.000	90	1421429	20.0	20.9	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	940456	20.0	20.6	
74 Tetrachloroethene	164	7.117	7.117	0.000	96	1049416	20.0	20.9	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	93	1663194	20.0	20.7	
76 2-Hexanone	43	7.188	7.188	0.000	96	1487023	40.0	42.4	
79 Chlorodibromomethane	129	7.342	7.342	0.000	90	1084488	20.0	22.7	
80 Ethylene Dibromide	107	7.461	7.461	0.000	99	999728	20.0	20.4	
82 Chlorobenzene	112	7.900	7.900	0.000	95	3072375	20.0	20.5	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	95	1113186	20.0	21.0	
84 Ethylbenzene	106	7.995	7.995	0.000	98	1624425	20.0	20.6	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	3890600	20.0	20.8	
86 o-Xylene	106	8.481	8.481	0.000	96	1968397	20.0	20.7	
87 Styrene	104	8.493	8.493	0.000	93	3394736	20.0	21.4	
88 Bromoform	173	8.682	8.682	0.000	98	770158	20.0	20.3	
89 Isopropylbenzene	105	8.825	8.825	0.000	96	4695119	20.0	20.9	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	1238040	20.0	20.3	
92 Bromobenzene	156	9.145	9.133	0.012	89	1450127	20.0	20.4	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	84	423192	20.0	20.0	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	75	276245	20.0	31.7	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	1274023	20.0	20.4	
97 2-Chlorotoluene	126	9.323	9.323	0.000	98	1188057	20.0	20.3	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	3784392	20.0	20.8	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	3844885	20.0	20.3	
101 tert-Butylbenzene	119	9.714	9.714	0.000	92	3285832	20.0	20.2	
103 1,2,4-Trimethylbenzene	105	9.762	9.762	0.000	94	3917785	20.0	20.5	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
105 sec-Butylbenzene	105	9.928	9.928	0.000	93	4155710	20.0	20.8	
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	98	2462678	20.0	20.1	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	97	3739399	20.0	20.9	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	97	2527274	20.0	19.9	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	2918965	20.0	20.6	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	99	2381785	20.0	20.0	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	93	306515	20.0	22.2	
115 1,2,4-Trichlorobenzene	180	12.110	12.110	0.000	94	1510157	20.0	20.0	
116 Hexachlorobutadiene	225	12.276	12.276	0.000	93	696597	20.0	20.4	
117 Naphthalene	128	12.359	12.359	0.000	96	3879317	20.0	20.5	
118 1,2,3-Trichlorobenzene	180	12.608	12.608	0.000	96	1364016	20.0	20.1	
S 127 1,2-Dichloroethene, Total	96				0			40.0	
S 128 1,3-Dichloropropene, Total	75				0			44.0	
S 129 Xylenes, Total	106				0		40.0	41.5	
S 130 Trihalomethanes, Total	1				0		80.0	84.8	
S 157 Total BTEX	1		0.000				100.0	ND	

Reagents:

vm50ss_stk_00079	Amount Added: 16.00	Units: uL
VM50IS_00072	Amount Added: 1.00	Units: uL
VMRPRIMW_00318	Amount Added: 16.00	Units: uL
VMAROLISTDW_00281	Amount Added: 16.00	Units: uL
VMRGAS_00278	Amount Added: 16.00	Units: uL

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8411.D

Injection Date: 21-Jan-2019 11:59:30

Instrument ID: A3UX15

Operator ID:

Lims ID: STD8260 L5

Worklist Smp#: 3

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 2

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

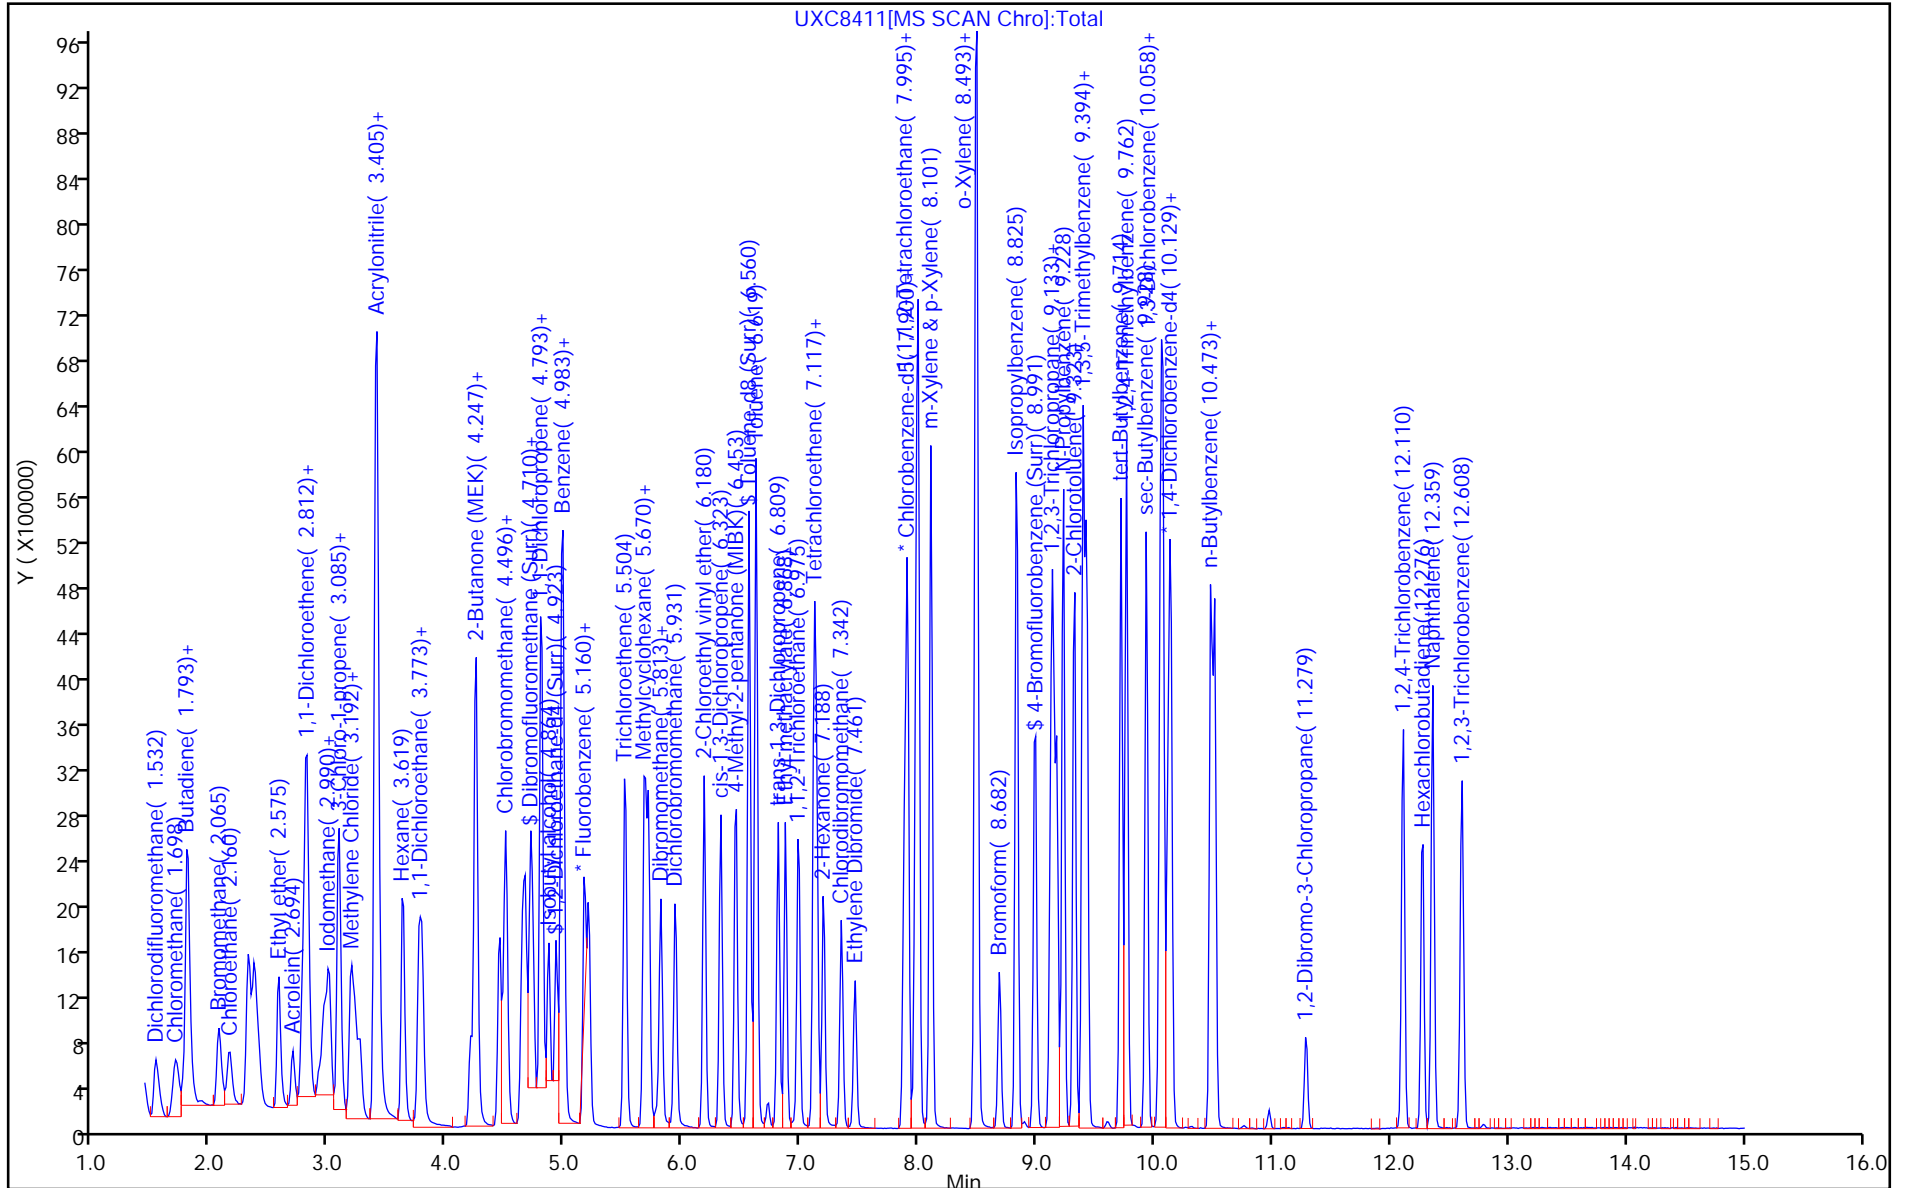

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8412.D
 Lims ID: STD8260 L4
 Client ID:
 Sample Type: ICIS Calib Level: 4
 Inject. Date: 21-Jan-2019 12:21:30 ALS Bottle#: 3 Worklist Smp#: 4
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-004
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:09:43 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

First Level Reviewer: evansle

Date: 21-Jan-2019 12:44:31

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1873821	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	85	1485792	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	831741	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	447792	10.0	10.1	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	573781	10.0	10.1	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	1816996	10.0	10.1	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	96	649263	10.0	10.1	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	593761	10.0	10.3	
10 Chloromethane	50	1.686	1.686	0.000	99	585358	10.0	9.96	
11 Vinyl chloride	62	1.781	1.781	0.000	98	574312	10.0	10.6	
12 Butadiene	54	1.793	1.793	0.000	98	698736	10.0	9.83	
13 Bromomethane	94	2.054	2.054	0.000	91	423055	10.0	9.78	
14 Chloroethane	64	2.137	2.137	0.000	100	372694	10.0	9.74	
15 Dichlorofluoromethane	67	2.303	2.303	0.000	97	910063	10.0	9.52	
16 Trichlorofluoromethane	101	2.362	2.362	0.000	99	855986	10.0	10.5	
17 Ethyl ether	59	2.563	2.563	0.000	91	419544	10.0	9.69	
18 Acrolein	56	2.694	2.694	0.000	99	290454	50.0	48.9	
19 1,1-Dichloroethene	96	2.777	2.777	0.000	98	516876	10.0	9.18	
20 1,1,2-Trichloro-1,2,2-trif	151	2.789	2.789	0.000	87	462285	10.0	10.0	
22 Acetone	58	2.812	2.812	0.000	99	89168	20.0	19.7	
23 Iodomethane	142	2.931	2.931	0.000	98	909454	10.0	10.4	
24 Carbon disulfide	76	2.990	2.990	0.000	100	1445567	10.0	9.97	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	88	317161	10.0	9.97	
27 Methyl acetate	43	3.085	3.085	0.000	97	723073	20.0	18.8	
28 Methylene Chloride	84	3.180	3.180	0.000	92	580808	10.0	10.0	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	328142	100.0	86.3	
32 Acrylonitrile	53	3.394	3.394	0.000	98	1699336	100.0	94.3	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	97	500088	10.0	9.55	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	1439491	10.0	9.81	
33 Hexane	86	3.619	3.619	0.000	95	104918	10.0	9.55	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	832192	10.0	9.83	
36 Vinyl acetate	43	3.785	3.785	0.000	97	992089	10.0	10.2	
39 cis-1,2-Dichloroethene	96	4.235	4.235	0.000	81	565374	10.0	9.80	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	98	120010	20.0	19.3	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	70	120845	10.0	10.3	
45 Chlorobromomethane	128	4.449	4.449	0.000	88	275468	10.0	9.60	
46 Tetrahydrofuran	42	4.485	4.485	0.000	87	279158	20.0	18.0	
47 Chloroform	83	4.496	4.496	0.000	93	847597	10.0	9.82	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	98	689229	10.0	10.4	
49 Cyclohexane	56	4.710	4.710	0.000	91	742256	10.0	9.92	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	94	688186	10.0	9.80	
50 Carbon tetrachloride	117	4.805	4.805	0.000	96	648774	10.0	10.1	
52 Isobutyl alcohol	41	4.864	4.864	0.000	95	322275	250.0	223.9	
53 Benzene	78	4.971	4.971	0.000	96	2024145	10.0	9.68	
54 1,2-Dichloroethane	62	4.983	4.983	0.000	98	707702	10.0	9.89	
56 n-Heptane	100	5.160	5.160	0.000	93	101813	10.0	10.2	
58 Trichloroethene	130	5.504	5.504	0.000	96	593061	10.0	9.77	
60 Methylcyclohexane	83	5.670	5.670	0.000	90	654672	10.0	9.91	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	94	483376	10.0	9.96	
63 Dibromomethane	93	5.813	5.813	0.000	89	317664	10.0	9.87	
64 1,4-Dioxane	88	5.813	5.813	0.000	33	71764	200.0	180.7	
65 Dichlorobromomethane	83	5.931	5.931	0.000	99	637533	10.0	9.98	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	640886	20.0	19.6	
68 cis-1,3-Dichloropropene	75	6.323	6.323	0.000	95	746312	10.0	10.1	
69 4-Methyl-2-pentanone (MIBK)	43	6.441	6.441	0.000	97	970866	20.0	19.3	
70 Toluene	91	6.619	6.619	0.000	98	2172974	10.0	9.91	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	94	706531	10.0	10.2	
72 Ethyl methacrylate	69	6.868	6.868	0.000	89	647349	10.0	9.81	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	437245	10.0	9.87	
74 Tetrachloroethene	164	7.117	7.117	0.000	96	482895	10.0	9.95	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	93	779324	10.0	10.0	
76 2-Hexanone	43	7.188	7.188	0.000	97	666112	20.0	19.6	
79 Chlorodibromomethane	129	7.342	7.342	0.000	90	469828	10.0	10.1	
80 Ethylene Dibromide	107	7.461	7.461	0.000	98	469490	10.0	9.90	
82 Chlorobenzene	112	7.900	7.900	0.000	95	1441533	10.0	9.92	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	94	522591	10.0	10.2	
84 Ethylbenzene	106	7.995	7.995	0.000	98	758362	10.0	9.92	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	1818169	10.0	10.0	
86 o-Xylene	106	8.481	8.481	0.000	96	918350	10.0	9.99	
87 Styrene	104	8.493	8.493	0.000	93	1550959	10.0	10.1	
88 Bromoform	173	8.682	8.682	0.000	98	306750	10.0	8.74	
89 Isopropylbenzene	105	8.825	8.825	0.000	95	2200366	10.0	10.1	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	577712	10.0	9.80	
92 Bromobenzene	156	9.133	9.133	0.000	89	678570	10.0	9.86	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	75	66363	10.0	7.87	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	83	201010	10.0	9.79	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	601438	10.0	9.92	
97 2-Chlorotoluene	126	9.323	9.323	0.000	98	555062	10.0	9.78	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	1766210	10.0	10.0	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	1798133	10.0	9.80	
101 tert-Butylbenzene	119	9.714	9.714	0.000	91	1551899	10.0	9.83	
103 1,2,4-Trimethylbenzene	105	9.762	9.762	0.000	94	1848645	10.0	9.98	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
105 sec-Butylbenzene	105	9.928	9.928	0.000	94	1935865	10.0	10.0	
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	99	1168047	10.0	9.86	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	97	1751242	10.0	10.1	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	97	1199185	10.0	9.76	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	1384405	10.0	10.1	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	99	1159176	10.0	10.0	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	91	138143	10.0	10.3	
115 1,2,4-Trichlorobenzene	180	12.110	12.110	0.000	93	739836	10.0	10.1	
116 Hexachlorobutadiene	225	12.276	12.276	0.000	93	359850	10.0	9.75	
117 Naphthalene	128	12.359	12.359	0.000	96	1891386	10.0	10.3	
118 1,2,3-Trichlorobenzene	180	12.608	12.608	0.000	95	663704	10.0	10.1	
S 129 Xylenes, Total	106				0		20.0	20.0	
S 157 Total BTEX	1		0.000				50.0	ND	
S 130 Trihalomethanes, Total	1				0		40.0	38.7	

Reagents:

VM50IS_00072	Amount Added: 1.00	Units: uL
vm50ss_stk_00079	Amount Added: 8.00	Units: uL
VMRPRIMW_00318	Amount Added: 8.00	Units: uL
VMAROLISTDW_00281	Amount Added: 8.00	Units: uL
VMRGAS_00278	Amount Added: 8.00	Units: uL

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8412.D

Injection Date: 21-Jan-2019 12:21:30

Instrument ID: A3UX15

Operator ID:

Lims ID: STD8260 L4

Worklist Smp#: 4

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 3

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

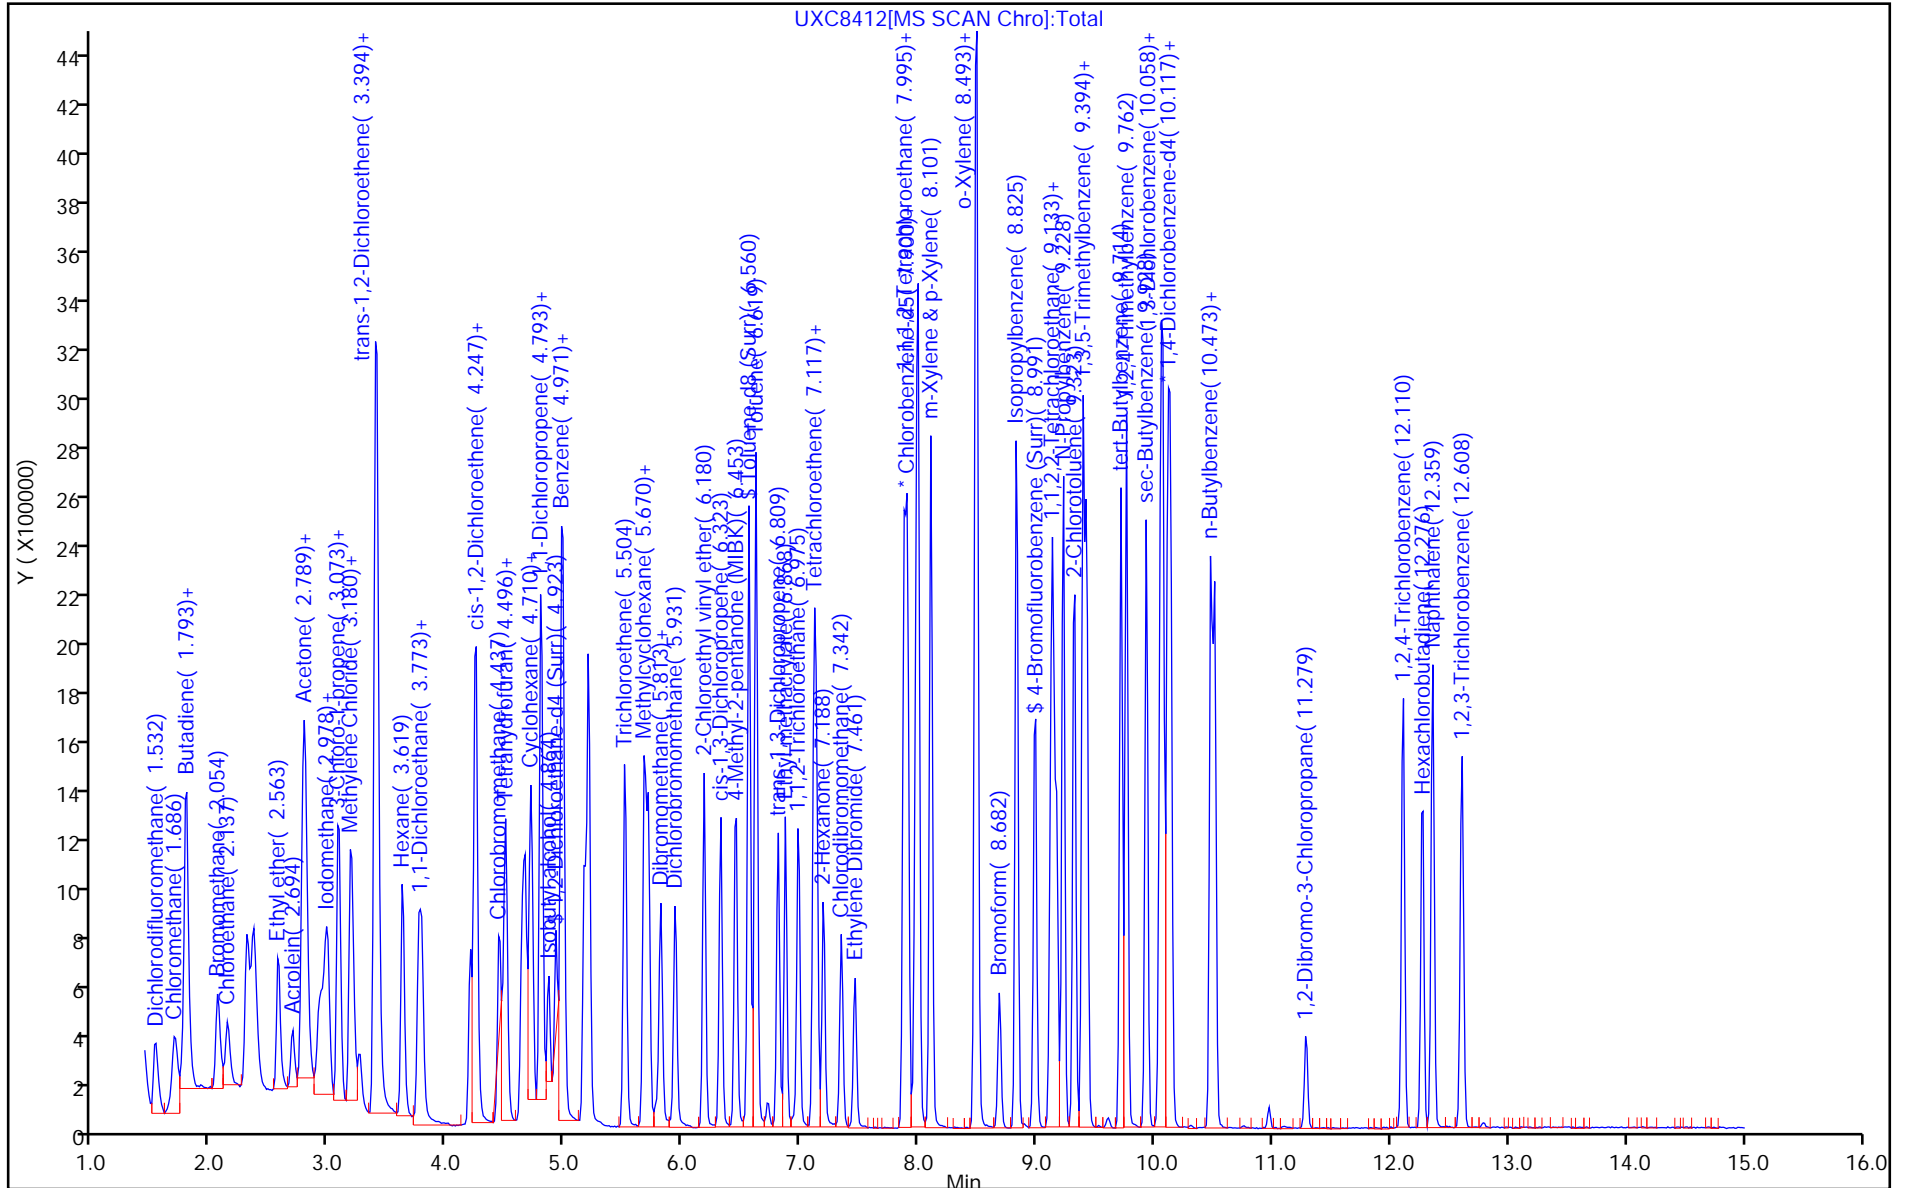

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8413.D
 Lims ID: STD8260 L3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 21-Jan-2019 12:43:30 ALS Bottle#: 4 Worklist Smp#: 5
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-005
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:09:48 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

First Level Reviewer: evansle

Date: 21-Jan-2019 13:20:00

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1838760	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	85	1476200	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	809369	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	225163	5.00	5.18	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	288691	5.00	5.16	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	912990	5.00	5.10	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	96	328418	5.00	5.13	
9 Dichlorodifluoromethane	85	1.520	1.532	-0.012	99	296202	5.00	5.24	
10 Chloromethane	50	1.686	1.686	0.000	99	276149	5.00	4.79	
11 Vinyl chloride	62	1.781	1.781	0.000	67	261470	5.00	4.93	
12 Butadiene	54	1.793	1.793	0.000	95	361713	5.00	5.18	
13 Bromomethane	94	2.053	2.054	-0.001	91	198900	5.00	4.69	
14 Chloroethane	64	2.136	2.137	-0.001	100	182320	5.00	4.86	
15 Dichlorofluoromethane	67	2.302	2.303	-0.001	98	471934	5.00	5.03	
16 Trichlorofluoromethane	101	2.362	2.362	0.000	98	408598	5.00	5.12	
17 Ethyl ether	59	2.563	2.563	0.000	90	212667	5.00	5.01	
18 Acrolein	56	2.694	2.694	0.000	99	144856	25.0	24.9	
19 1,1-Dichloroethene	96	2.789	2.777	0.012	98	277159	5.00	5.02	
20 1,1,2-Trichloro-1,2,2-trif	151	2.789	2.789	0.000	87	228498	5.00	5.04	
22 Acetone	58	2.812	2.812	0.000	99	50751	10.0	10.4	
23 Iodomethane	142	2.943	2.931	0.012	98	446819	5.00	5.20	
24 Carbon disulfide	76	2.990	2.990	0.000	100	742305	5.00	5.21	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	88	154763	5.00	4.96	
27 Methyl acetate	43	3.085	3.085	0.000	98	380996	10.0	10.1	
28 Methylene Chloride	84	3.180	3.180	0.000	93	338417	5.00	4.93	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	184510	50.0	49.5	
32 Acrylonitrile	53	3.393	3.394	-0.001	98	868795	50.0	49.1	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	714788	5.00	4.96	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	98	251570	5.00	4.89	
33 Hexane	86	3.631	3.619	0.012	94	51427	5.00	4.77	

Compound	Sig	RT (min.)	Exp RT (min.)	Diff RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	409730	5.00	4.93	
36 Vinyl acetate	43	3.785	3.785	0.000	97	476538	5.00	4.99	
39 cis-1,2-Dichloroethene	96	4.235	4.235	0.000	80	278759	5.00	4.92	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	68	58586	5.00	5.11	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	99	59681	10.0	9.76	
45 Chlorobromomethane	128	4.449	4.449	0.000	89	140018	5.00	4.97	
46 Tetrahydrofuran	42	4.484	4.485	-0.001	88	150812	10.0	9.91	
47 Chloroform	83	4.496	4.496	0.000	93	422474	5.00	4.99	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	97	334136	5.00	5.12	
49 Cyclohexane	56	4.710	4.710	0.000	90	368473	5.00	5.02	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	93	343617	5.00	4.99	
50 Carbon tetrachloride	117	4.805	4.805	0.000	96	318843	5.00	5.04	
52 Isobutyl alcohol	41	4.864	4.864	0.000	94	177736	125.0	125.8	
53 Benzene	78	4.971	4.971	0.000	96	1016161	5.00	4.95	
54 1,2-Dichloroethane	62	4.982	4.983	-0.001	97	350758	5.00	4.99	
56 n-Heptane	100	5.160	5.160	0.000	93	48491	5.00	4.96	
58 Trichloroethene	130	5.504	5.504	0.000	96	296310	5.00	4.97	
60 Methylcyclohexane	83	5.670	5.670	0.000	89	326169	5.00	5.03	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	94	239856	5.00	5.04	
64 1,4-Dioxane	88	5.813	5.813	0.000	33	39232	100.0	103.2	M
63 Dibromomethane	93	5.813	5.813	0.000	89	157375	5.00	4.99	
65 Dichlorobromomethane	83	5.931	5.931	0.000	99	306036	5.00	4.88	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	319533	10.0	9.96	
68 cis-1,3-Dichloropropene	75	6.322	6.323	-0.001	94	356486	5.00	4.92	
69 4-Methyl-2-pentanone (MIBK)	43	6.441	6.441	0.000	97	495239	10.0	10.1	
70 Toluene	91	6.619	6.619	0.000	98	1080197	5.00	4.96	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	94	333930	5.00	4.87	
72 Ethyl methacrylate	69	6.868	6.868	0.000	89	316654	5.00	4.83	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	218933	5.00	4.97	
74 Tetrachloroethene	164	7.117	7.117	0.000	96	241473	5.00	5.01	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	92	378264	5.00	4.89	
76 2-Hexanone	43	7.188	7.188	0.000	97	337296	10.0	10.0	
79 Chlorodibromomethane	129	7.342	7.342	0.000	89	222991	5.00	4.85	
80 Ethylene Dibromide	107	7.461	7.461	0.000	97	237763	5.00	5.05	
82 Chlorobenzene	112	7.900	7.900	0.000	95	714138	5.00	4.95	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	93	253355	5.00	4.97	
84 Ethylbenzene	106	7.995	7.995	0.000	98	374569	5.00	4.93	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	872988	5.00	4.84	
86 o-Xylene	106	8.481	8.481	0.000	96	449671	5.00	4.92	
87 Styrene	104	8.493	8.493	0.000	94	754758	5.00	4.94	
88 Bromoform	173	8.682	8.682	0.000	98	138461	5.00	4.32	
89 Isopropylbenzene	105	8.825	8.825	0.000	96	1070139	5.00	4.95	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	283791	5.00	4.95	
92 Bromobenzene	156	9.133	9.133	0.000	89	330598	5.00	4.94	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	83	99350	5.00	4.97	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	62	23872	5.00	2.91	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	290505	5.00	4.93	
97 2-Chlorotoluene	126	9.323	9.323	0.000	97	275264	5.00	4.99	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	840604	5.00	4.90	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	881245	5.00	4.94	
101 tert-Butylbenzene	119	9.714	9.714	0.000	92	749194	5.00	4.88	
103 1,2,4-Trimethylbenzene	105	9.761	9.762	-0.001	94	876431	5.00	4.86	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
105 sec-Butylbenzene	105	9.927	9.928	-0.001	94	937713	5.00	4.98	
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	98	572540	5.00	4.96	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	97	830781	5.00	4.93	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	97	582208	5.00	4.87	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	659506	5.00	4.94	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	99	556492	5.00	4.96	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	90	65389	5.00	5.01	
115 1,2,4-Trichlorobenzene	180	12.109	12.110	-0.001	94	356465	5.00	5.01	
116 Hexachlorobutadiene	225	12.275	12.276	-0.001	94	175613	5.00	4.68	
117 Naphthalene	128	12.358	12.359	-0.001	96	926474	5.00	5.18	
118 1,2,3-Trichlorobenzene	180	12.607	12.608	-0.001	96	324635	5.00	5.08	
S 127 1,2-Dichloroethene, Total	96				0			9.82	
S 128 1,3-Dichloropropene, Total	75				0			9.78	
S 129 Xylenes, Total	106				0		10.0	9.77	
S 130 Trihalomethanes, Total	1				0		20.0	19.0	
S 157 Total BTEX	1		0.000				25.0	ND	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

VM50IS_00072	Amount Added: 1.00	Units: uL
vm50ss_stk_00079	Amount Added: 4.00	Units: uL
VMRPRIMW_00318	Amount Added: 4.00	Units: uL
VMAROLISTDW_00281	Amount Added: 4.00	Units: uL
VMRGAS_00278	Amount Added: 4.00	Units: uL

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8413.D

Injection Date: 21-Jan-2019 12:43:30

Instrument ID: A3UX15

Operator ID:

Lims ID: STD8260 L3

Worklist Smp#: 5

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 4

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

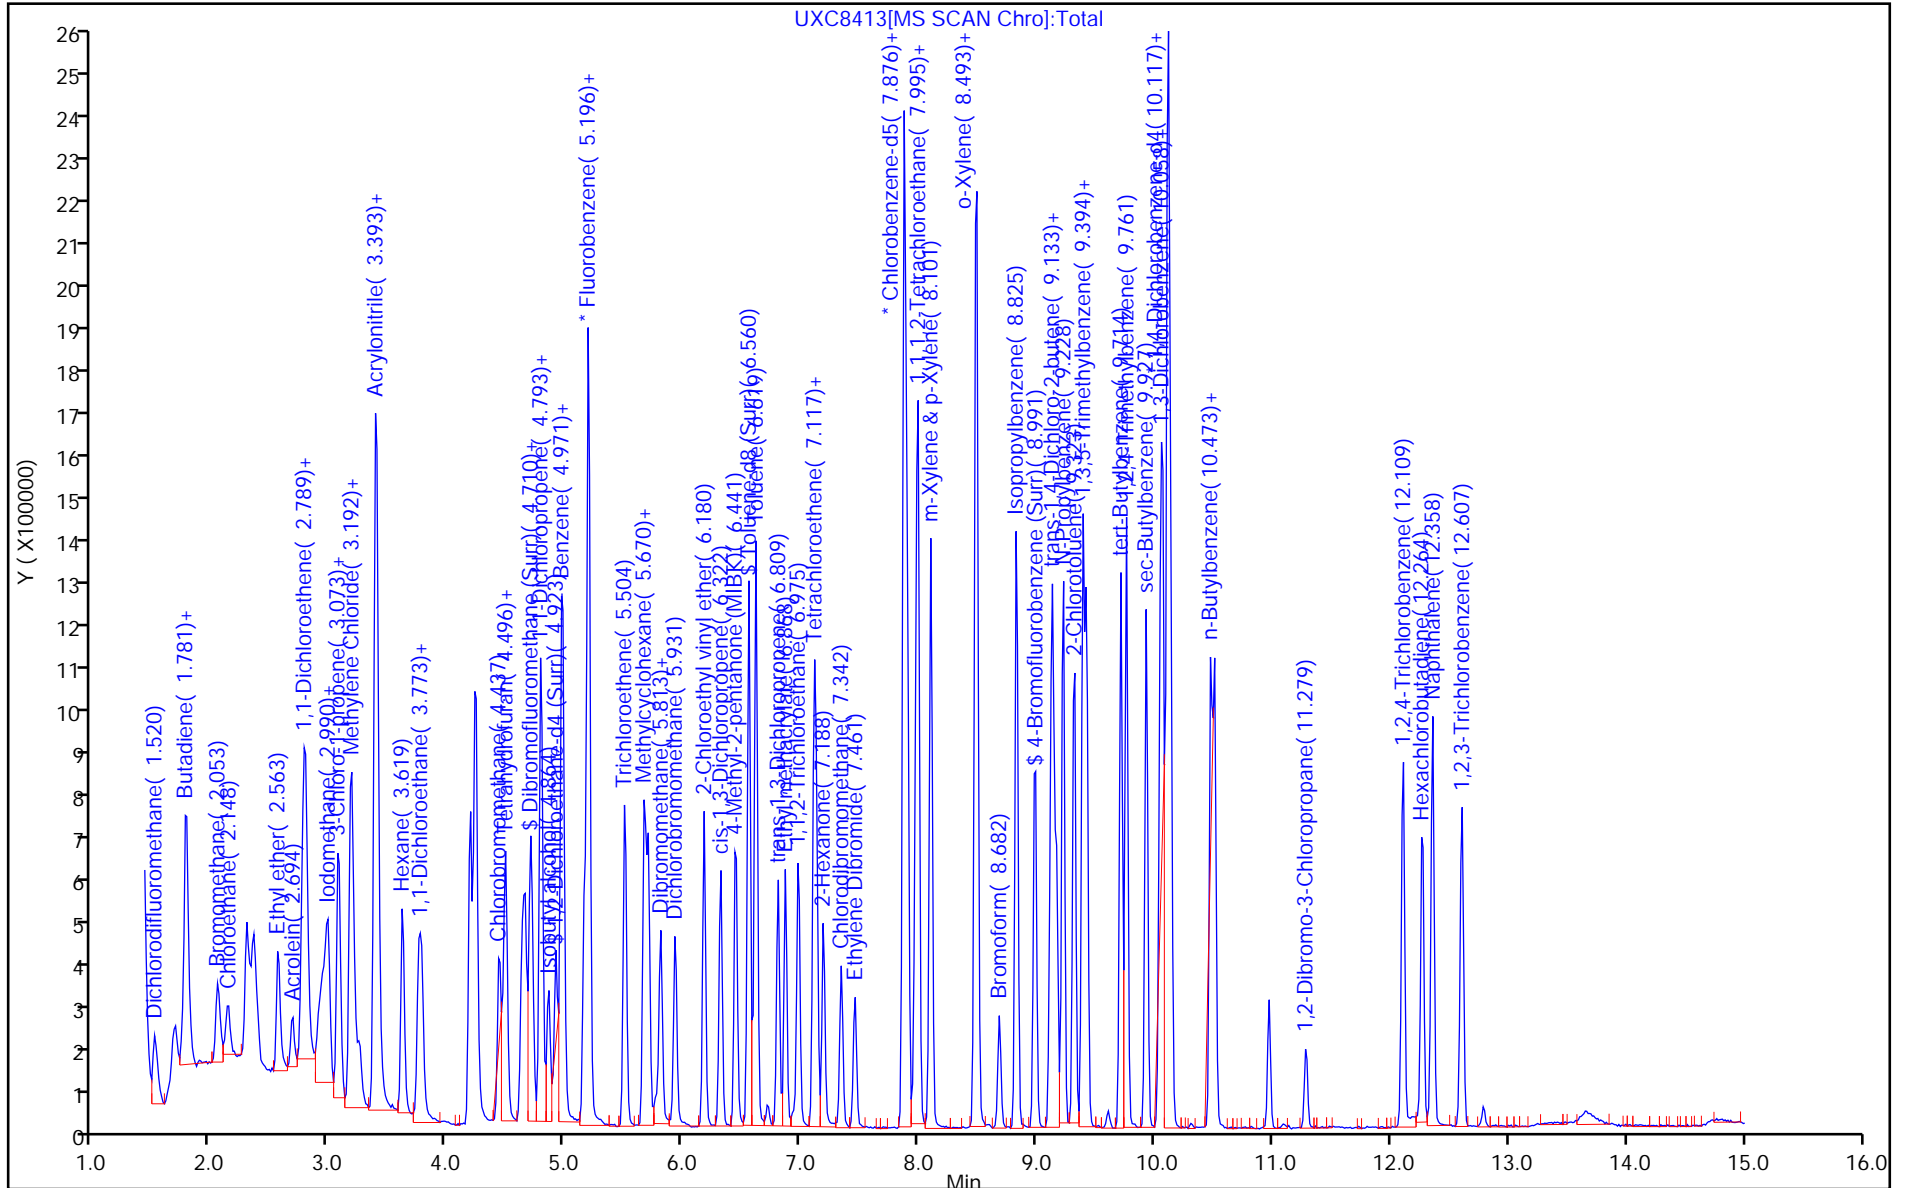

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8413.D
Injection Date: 21-Jan-2019 12:43:30 Instrument ID: A3UX15
Lims ID: STD8260 L3
Client ID:
Operator ID:
Purge Vol: 5.000 mL
Method: 8260_15
Column: DB-624 (0.18 mm)


ALS Bottle#: 4 Worklist Smp#: 5
Dil. Factor: 1.0000
Limit Group: MSV 8260B ICAL
Detector MS SCAN

64 1,4-Dioxane, CAS: 123-91-1

Signal: 1


RT: 5.81
Area: 29665
Amount: 80.472140
Amount Units: ug/l

Processing Integration Results

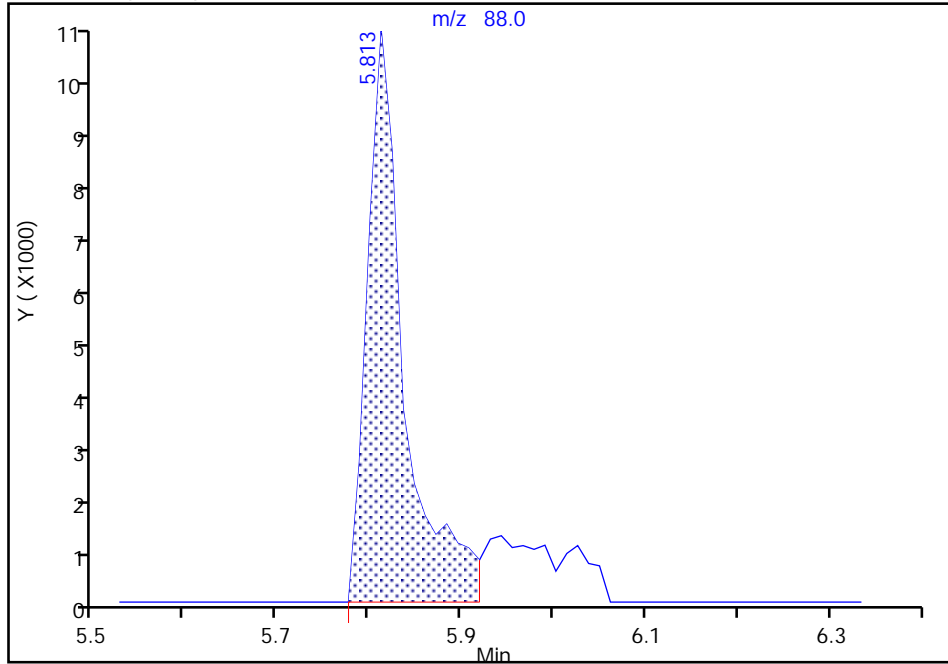

RT: 5.81
Area: 39232
Amount: 103.2242
Amount Units: ug/l

Manual Integration Results

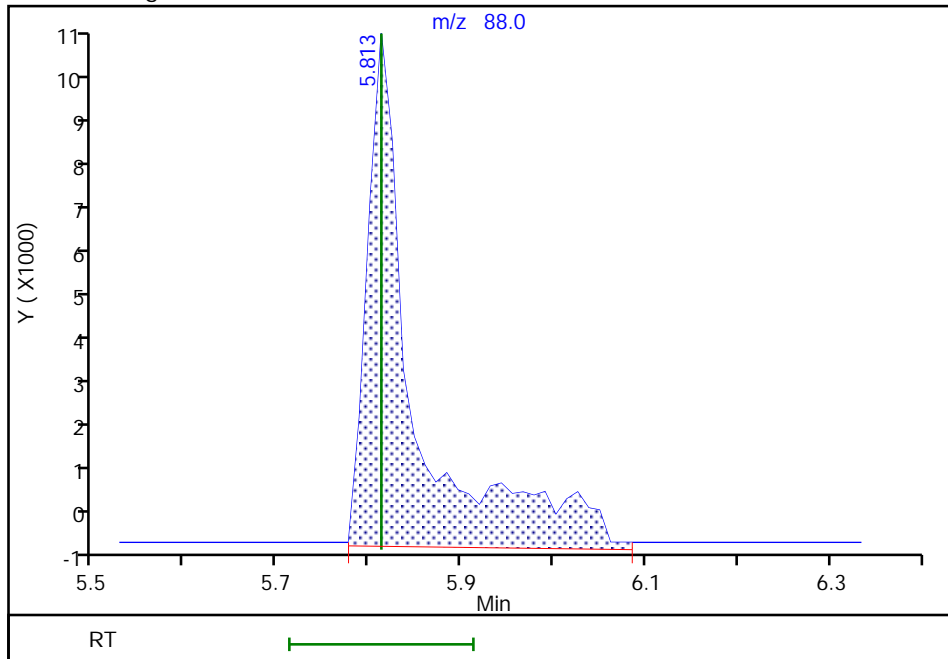

Reviewer: evansle, 21-Jan-2019 13:18:53

Audit Action: Manually Integrated

Audit Reason: Baseline



TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8414.D
 Lims ID: STD8260 L2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 21-Jan-2019 13:05:30 ALS Bottle#: 5 Worklist Smp#: 6
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-006
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:09:53 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

First Level Reviewer: evansle

Date: 21-Jan-2019 13:21:36

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1827101	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1454104	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	793660	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	94	80448	2.00	1.86	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	106482	2.00	1.92	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	333303	2.00	1.89	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	95	120695	2.00	1.91	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	112693	2.00	2.01	
10 Chloromethane	50	1.698	1.686	0.012	99	119628	2.00	2.09	
11 Vinyl chloride	62	1.793	1.781	0.012	62	104647	2.00	1.99	
12 Butadiene	54	1.793	1.793	0.000	96	148568	2.00	2.14	
13 Bromomethane	94	2.065	2.054	0.011	91	100403	2.00	2.38	
14 Chloroethane	64	2.148	2.137	0.011	100	82718	2.00	2.22	
15 Dichlorofluoromethane	67	2.314	2.303	0.011	98	201291	2.00	2.16	
16 Trichlorofluoromethane	101	2.362	2.362	0.000	97	157640	2.00	1.99	
17 Ethyl ether	59	2.575	2.563	0.012	90	87432	2.00	2.07	
18 Acrolein	56	2.694	2.694	0.000	99	55282	10.0	9.55	
19 1,1-Dichloroethene	96	2.801	2.777	0.024	98	120279	2.00	2.19	
20 1,1,2-Trichloro-1,2,2-trif	151	2.801	2.789	0.012	77	91700	2.00	2.03	
22 Acetone	58	2.812	2.812	0.000	98	23252	4.00	3.50	
23 Iodomethane	142	2.955	2.931	0.024	98	156089	2.00	1.83	
24 Carbon disulfide	76	3.002	2.990	0.012	100	283969	2.00	2.01	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	86	58477	2.00	1.88	
27 Methyl acetate	43	3.085	3.085	0.000	97	150240	4.00	4.01	
28 Methylene Chloride	84	3.180	3.180	0.000	96	198393	2.00	1.89	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	82343	20.0	22.2	
32 Acrylonitrile	53	3.393	3.394	-0.001	100	352291	20.0	20.0	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	96	103155	2.00	2.02	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	285516	2.00	1.99	
33 Hexane	86	3.631	3.619	0.012	93	22194	2.00	2.07	

Compound	Sig	RT (min.)	Exp RT (min.)	Diff RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
34 1,1-Dichloroethane	63	3.761	3.761	0.000	96	166930	2.00	2.02	
36 Vinyl acetate	43	3.785	3.785	0.000	97	177639	2.00	1.87	
39 cis-1,2-Dichloroethene	96	4.247	4.235	0.012	81	116480	2.00	2.07	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	72	24387	4.00	4.01	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	60	21907	2.00	1.92	
45 Chlorobromomethane	128	4.449	4.449	0.000	90	56716	2.00	2.03	
46 Tetrahydrofuran	42	4.484	4.485	-0.001	86	62314	4.00	4.12	
47 Chloroform	83	4.496	4.496	0.000	94	169874	2.00	2.02	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	97	130349	2.00	2.01	
49 Cyclohexane	56	4.710	4.710	0.000	90	144320	2.00	1.98	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	94	140972	2.00	2.06	
50 Carbon tetrachloride	117	4.805	4.805	0.000	97	124489	2.00	1.98	
52 Isobutyl alcohol	41	4.864	4.864	0.000	96	73133	50.0	52.1	
53 Benzene	78	4.971	4.971	0.000	95	412777	2.00	2.02	
54 1,2-Dichloroethane	62	4.983	4.983	0.000	98	142414	2.00	2.04	
56 n-Heptane	100	5.160	5.160	0.000	92	19095	2.00	1.96	
58 Trichloroethene	130	5.504	5.504	0.000	96	120531	2.00	2.04	
60 Methylcyclohexane	83	5.670	5.670	0.000	90	127322	2.00	1.98	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	94	97800	2.00	2.07	
63 Dibromomethane	93	5.813	5.813	0.000	89	65366	2.00	2.08	
64 1,4-Dioxane	88	5.813	5.813	0.000	37	14227	40.0	41.3	
65 Dichlorobromomethane	83	5.931	5.931	0.000	98	121869	2.00	1.96	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	123378	4.00	3.87	
68 cis-1,3-Dichloropropene	75	6.323	6.323	0.000	94	138202	2.00	1.92	
69 4-Methyl-2-pentanone (MIBK)	43	6.453	6.441	0.012	96	187250	4.00	3.83	
70 Toluene	91	6.619	6.619	0.000	98	428381	2.00	2.00	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	95	125256	2.00	1.85	
72 Ethyl methacrylate	69	6.868	6.868	0.000	89	129112	2.00	2.00	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	87521	2.00	2.02	
74 Tetrachloroethene	164	7.117	7.117	0.000	96	95990	2.00	2.02	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	92	153833	2.00	2.02	
76 2-Hexanone	43	7.188	7.188	0.000	97	135481	4.00	4.08	
79 Chlorodibromomethane	129	7.342	7.342	0.000	90	82891	2.00	1.83	
80 Ethylene Dibromide	107	7.461	7.461	0.000	98	91132	2.00	1.96	
82 Chlorobenzene	112	7.900	7.900	0.000	97	286159	2.00	2.01	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	93	95060	2.00	1.89	
84 Ethylbenzene	106	7.995	7.995	0.000	98	146696	2.00	1.96	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	351787	2.00	1.98	
86 o-Xylene	106	8.481	8.481	0.000	96	176986	2.00	1.97	
87 Styrene	104	8.493	8.493	0.000	91	289260	2.00	1.92	
88 Bromoform	173	8.682	8.682	0.000	97	51580	2.00	2.03	
89 Isopropylbenzene	105	8.825	8.825	0.000	95	416807	2.00	1.96	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	112833	2.00	2.01	
92 Bromobenzene	156	9.133	9.133	0.000	89	131876	2.00	2.01	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	67	16039	2.00	1.99	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	86	40526	2.00	2.07	
96 N-Propylbenzene	120	9.228	9.228	0.000	98	117423	2.00	2.03	
97 2-Chlorotoluene	126	9.323	9.323	0.000	98	107735	2.00	1.99	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	332591	2.00	1.98	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	356628	2.00	2.04	
101 tert-Butylbenzene	119	9.714	9.714	0.000	92	300630	2.00	2.00	
103 1,2,4-Trimethylbenzene	105	9.762	9.762	0.000	94	359918	2.00	2.04	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
105 sec-Butylbenzene	105	9.928	9.928	0.000	94	373619	2.00	2.02	
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	98	229119	2.00	2.03	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	96	334169	2.00	2.02	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	97	241629	2.00	2.06	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	263153	2.00	2.01	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	98	224899	2.00	2.04	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	88	24334	2.00	1.90	
115 1,2,4-Trichlorobenzene	180	12.109	12.110	-0.001	93	145803	2.00	2.09	
116 Hexachlorobutadiene	225	12.276	12.276	0.000	94	78276	2.00	2.11	
117 Naphthalene	128	12.359	12.359	0.000	96	348942	2.00	1.99	
118 1,2,3-Trichlorobenzene	180	12.608	12.608	0.000	95	131338	2.00	2.09	
S 127 1,2-Dichloroethene, Total	96				0			4.09	
S 128 1,3-Dichloropropene, Total	75				0			3.77	
S 129 Xylenes, Total	106				0		4.00	3.95	
S 157 Total BTEX	1		0.000				10.0	ND	
S 130 Trihalomethanes, Total	1				0		8.00	7.83	

Reagents:

VM50IS_00072	Amount Added: 1.00	Units: uL
vm50ss_stk_00079	Amount Added: 1.60	Units: uL
VMRPRIMW_00318	Amount Added: 1.60	Units: uL
VMAROLISTDW_00281	Amount Added: 1.60	Units: uL
VMRGAS_00278	Amount Added: 1.60	Units: uL

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8414.D

Injection Date: 21-Jan-2019 13:05:30

Instrument ID: A3UX15

Operator ID:

Lims ID: STD8260 L2

Worklist Smp#: 6

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 5

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

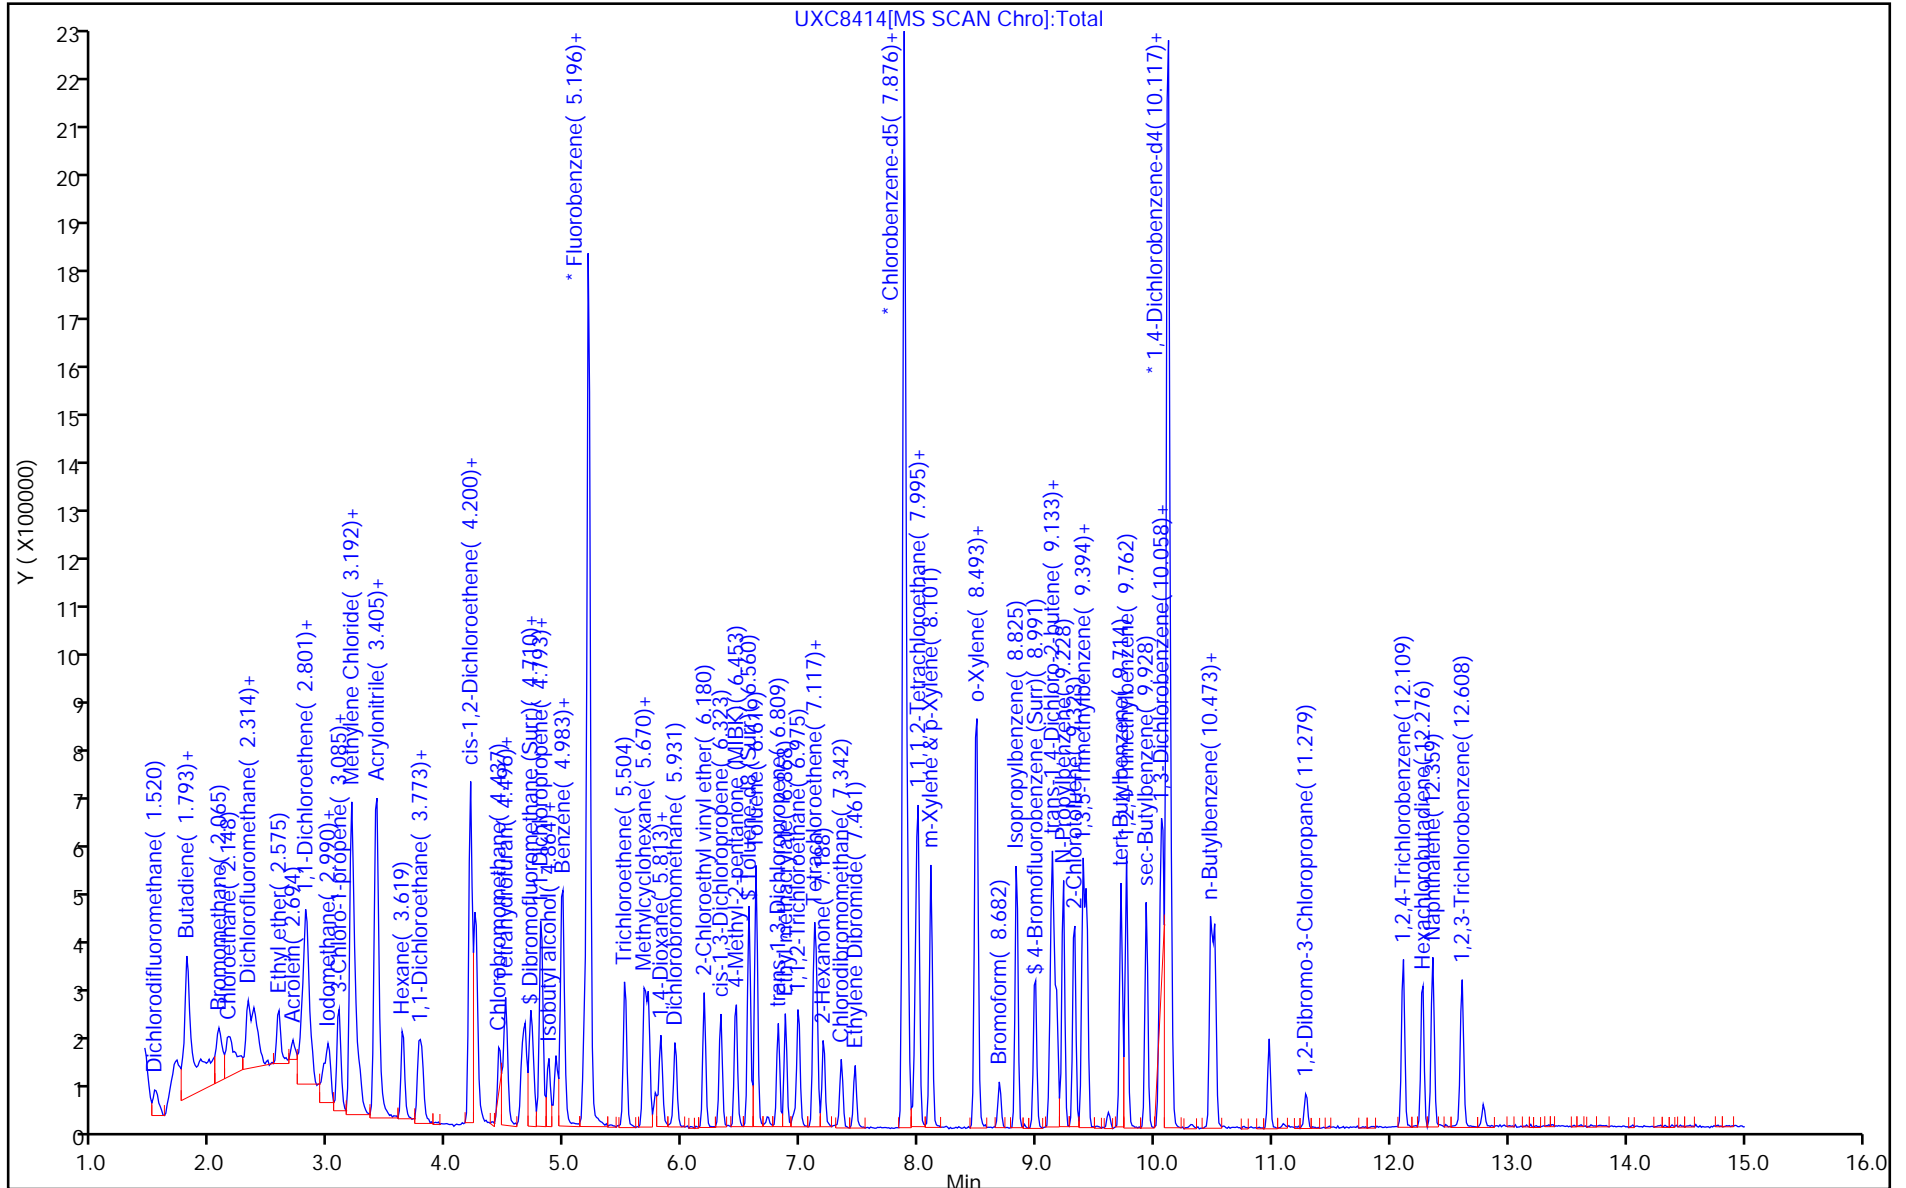

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8415.D
 Lims ID: STD8260 L1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 21-Jan-2019 13:26:30 ALS Bottle#: 6 Worklist Smp#: 7
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0083824-007
 Misc. Info.: C90121A-IC,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Sublist: chrom-8260_15*sub83
 Method: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 22-Jan-2019 09:09:57 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0303

First Level Reviewer: evansle

Date: 21-Jan-2019 13:51:17

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1764972	10.0	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1396761	10.0	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	94	755367	10.0	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	94	41840	1.00	1.00	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	55383	1.00	1.03	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	174193	1.00	1.03	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	95	60446	1.00	1.00	
9 Dichlorodifluoromethane	85	1.532	1.532	0.000	99	47729	1.00	0.8803	
10 Chloromethane	50	1.698	1.686	0.012	96	58046	1.00	1.05	
11 Vinyl chloride	62	1.793	1.781	0.012	72	57558	1.00	1.13	
12 Butadiene	54	1.793	1.793	0.000	95	71088	1.00	1.06	
13 Bromomethane	94	2.054	2.054	0.000	88	47411	1.00	1.16	
14 Chloroethane	64	2.137	2.137	0.000	99	40558	1.00	1.13	
15 Dichlorofluoromethane	67	2.303	2.303	0.000	97	103682	1.00	1.15	
16 Trichlorofluoromethane	101	2.350	2.362	-0.012	98	68568	1.00	0.8959	
17 Ethyl ether	59	2.575	2.563	0.012	91	44605	1.00	1.09	
18 Acrolein	56	2.694	2.694	0.000	97	32229	5.00	5.76	
19 1,1-Dichloroethene	96	2.777	2.777	0.000	98	57094	1.00	1.08	
20 1,1,2-Trichloro-1,2,2-trif	151	2.789	2.789	0.000	88	42550	1.00	0.9770	
22 Acetone	58	2.813	2.812	0.001	98	17181	2.00	2.11	
23 Iodomethane	142	2.931	2.931	0.000	99	93588	1.00	1.13	
24 Carbon disulfide	76	2.990	2.990	0.000	97	160687	1.00	1.18	
25 3-Chloro-1-propene	76	3.073	3.073	0.000	89	27003	1.00	0.9008	
27 Methyl acetate	43	3.085	3.085	0.000	98	79740	2.00	2.20	
28 Methylene Chloride	84	3.180	3.180	0.000	93	154915	1.00	1.05	
29 2-Methyl-2-propanol	59	3.263	3.263	0.000	99	36240	10.0	10.1	
32 Acrylonitrile	53	3.394	3.394	0.000	97	175156	10.0	10.3	
31 Methyl tert-butyl ether	73	3.405	3.405	0.000	96	139955	1.00	1.01	
30 trans-1,2-Dichloroethene	96	3.405	3.405	0.000	97	54736	1.00	1.11	
33 Hexane	86	3.619	3.619	0.000	94	10725	1.00	1.04	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
34 1,1-Dichloroethane	63	3.761	3.761	0.000	97	81126	1.00	1.02	
36 Vinyl acetate	43	3.785	3.785	0.000	97	88027	1.00	0.9595	
39 cis-1,2-Dichloroethene	96	4.236	4.235	0.001	80	57035	1.00	1.05	
40 2,2-Dichloropropane	97	4.247	4.247	0.000	42	11684	1.00	1.06	
41 2-Butanone (MEK)	72	4.247	4.247	0.000	57	12505	2.00	2.13	
45 Chlorobromomethane	128	4.437	4.449	-0.012	88	28543	1.00	1.06	
46 Tetrahydrofuran	42	4.485	4.485	0.000	86	31985	2.00	2.19	
47 Chloroform	83	4.496	4.496	0.000	93	83929	1.00	1.03	
48 1,1,1-Trichloroethane	97	4.662	4.662	0.000	98	63803	1.00	1.02	
49 Cyclohexane	56	4.710	4.710	0.000	91	68915	1.00	0.9779	
51 1,1-Dichloropropene	75	4.793	4.793	0.000	93	66437	1.00	1.00	
50 Carbon tetrachloride	117	4.805	4.805	0.000	97	56945	1.00	0.9377	
52 Isobutyl alcohol	41	4.864	4.864	0.000	95	31904	25.0	23.5	
53 Benzene	78	4.971	4.971	0.000	96	207184	1.00	1.05	
54 1,2-Dichloroethane	62	4.983	4.983	0.000	97	68031	1.00	1.01	
56 n-Heptane	100	5.161	5.160	0.000	80	8801	1.00	0.9370	a
58 Trichloroethene	130	5.504	5.504	0.000	95	59121	1.00	1.03	
60 Methylcyclohexane	83	5.670	5.670	0.000	88	60130	1.00	0.9667	
61 1,2-Dichloropropane	63	5.706	5.706	0.000	90	43707	1.00	0.9560	
64 1,4-Dioxane	88	5.825	5.813	0.012	33	5185	20.0	19.2	
63 Dibromomethane	93	5.813	5.813	0.000	86	31111	1.00	1.03	
65 Dichlorobromomethane	83	5.931	5.931	0.000	98	57382	1.00	0.9535	
67 2-Chloroethyl vinyl ether	63	6.180	6.180	0.000	93	61442	2.00	1.99	
68 cis-1,3-Dichloropropene	75	6.323	6.323	0.000	93	62099	1.00	0.8920	
69 4-Methyl-2-pentanone (MIBK)	43	6.453	6.441	0.012	98	98299	2.00	2.08	
70 Toluene	91	6.619	6.619	0.000	98	209687	1.00	1.02	
71 trans-1,3-Dichloropropene	75	6.809	6.809	0.000	94	57707	1.00	0.8893	
72 Ethyl methacrylate	69	6.868	6.868	0.000	90	61421	1.00	0.9899	
73 1,1,2-Trichloroethane	97	6.975	6.975	0.000	91	41853	1.00	1.00	
74 Tetrachloroethene	164	7.117	7.117	0.000	97	44889	1.00	0.9835	
75 1,3-Dichloropropane	76	7.129	7.129	0.000	92	72217	1.00	0.9861	
76 2-Hexanone	43	7.188	7.188	0.000	96	58616	2.00	1.84	
79 Chlorodibromomethane	129	7.342	7.342	0.000	89	36977	1.00	0.8497	
80 Ethylene Dibromide	107	7.461	7.461	0.000	97	45295	1.00	1.02	
82 Chlorobenzene	112	7.900	7.900	0.000	96	138107	1.00	1.01	
83 1,1,1,2-Tetrachloroethane	131	7.971	7.971	0.000	93	46702	1.00	0.9691	
84 Ethylbenzene	106	7.995	7.995	0.000	98	73699	1.00	1.03	
85 m-Xylene & p-Xylene	91	8.101	8.101	0.000	93	168049	1.00	0.9855	
86 o-Xylene	106	8.481	8.481	0.000	97	88147	1.00	1.02	
87 Styrene	104	8.493	8.493	0.000	93	137740	1.00	0.9520	
88 Bromoform	173	8.682	8.682	0.000	96	19867	1.00	1.20	
89 Isopropylbenzene	105	8.825	8.825	0.000	95	198841	1.00	0.9729	
93 1,1,2,2-Tetrachloroethane	83	9.121	9.121	0.000	97	54865	1.00	1.03	
92 Bromobenzene	156	9.133	9.133	0.000	90	63640	1.00	1.02	
94 1,2,3-Trichloropropane	110	9.169	9.169	0.000	85	18846	1.00	1.01	
95 trans-1,4-Dichloro-2-buten	53	9.169	9.169	0.000	62	3277	1.00	0.4279	
96 N-Propylbenzene	120	9.228	9.228	0.000	99	54874	1.00	1.00	
97 2-Chlorotoluene	126	9.323	9.323	0.000	97	53702	1.00	1.04	
98 1,3,5-Trimethylbenzene	105	9.394	9.394	0.000	94	160683	1.00	1.00	
99 4-Chlorotoluene	91	9.418	9.418	0.000	98	170473	1.00	1.02	
101 tert-Butylbenzene	119	9.714	9.714	0.000	92	141080	1.00	0.9843	
103 1,2,4-Trimethylbenzene	105	9.762	9.762	0.000	94	169136	1.00	1.01	

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	Cal Amt ug/l	OnCol Amt ug/l	Flags
105 sec-Butylbenzene	105	9.928	9.928	0.000	94	173094	1.00	0.9849	
106 1,3-Dichlorobenzene	146	10.046	10.046	0.000	97	113176	1.00	1.05	
107 4-Isopropyltoluene	119	10.070	10.070	0.000	95	154318	1.00	0.9808	
108 1,4-Dichlorobenzene	146	10.141	10.141	0.000	96	119243	1.00	1.07	
111 n-Butylbenzene	91	10.473	10.473	0.000	97	127428	1.00	1.02	
112 1,2-Dichlorobenzene	146	10.509	10.509	0.000	98	109056	1.00	1.04	
113 1,2-Dibromo-3-Chloropropan	157	11.291	11.291	0.000	84	10572	1.00	0.8688	
115 1,2,4-Trichlorobenzene	180	12.110	12.110	0.000	94	73453	1.00	1.11	
116 Hexachlorobutadiene	225	12.276	12.276	0.000	93	41867	1.00	1.20	
117 Naphthalene	128	12.359	12.359	0.000	96	172653	1.00	1.03	
118 1,2,3-Trichlorobenzene	180	12.608	12.608	0.000	95	65430	1.00	1.10	
S 127 1,2-Dichloroethene, Total	96				0			2.16	
S 128 1,3-Dichloropropene, Total	75				0			1.78	
S 129 Xylenes, Total	106				0		2.00	2.01	
S 130 Trihalomethanes, Total	1				0		4.00	4.03	
S 157 Total BTEX	1		0.000				5.00	ND	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

VM50IS_00072	Amount Added: 1.00	Units: uL
vm50ss_stk_00079	Amount Added: 0.80	Units: uL
VMRPRIMW_00318	Amount Added: 0.80	Units: uL
VMAROLISTDW_00281	Amount Added: 0.80	Units: uL
VMRGAS_00278	Amount Added: 0.80	Units: uL

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8415.D

Injection Date: 21-Jan-2019 13:26:30

Instrument ID: A3UX15

Operator ID:

Lims ID: STD8260 L1

Worklist Smp#: 7

Client ID:

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 6

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

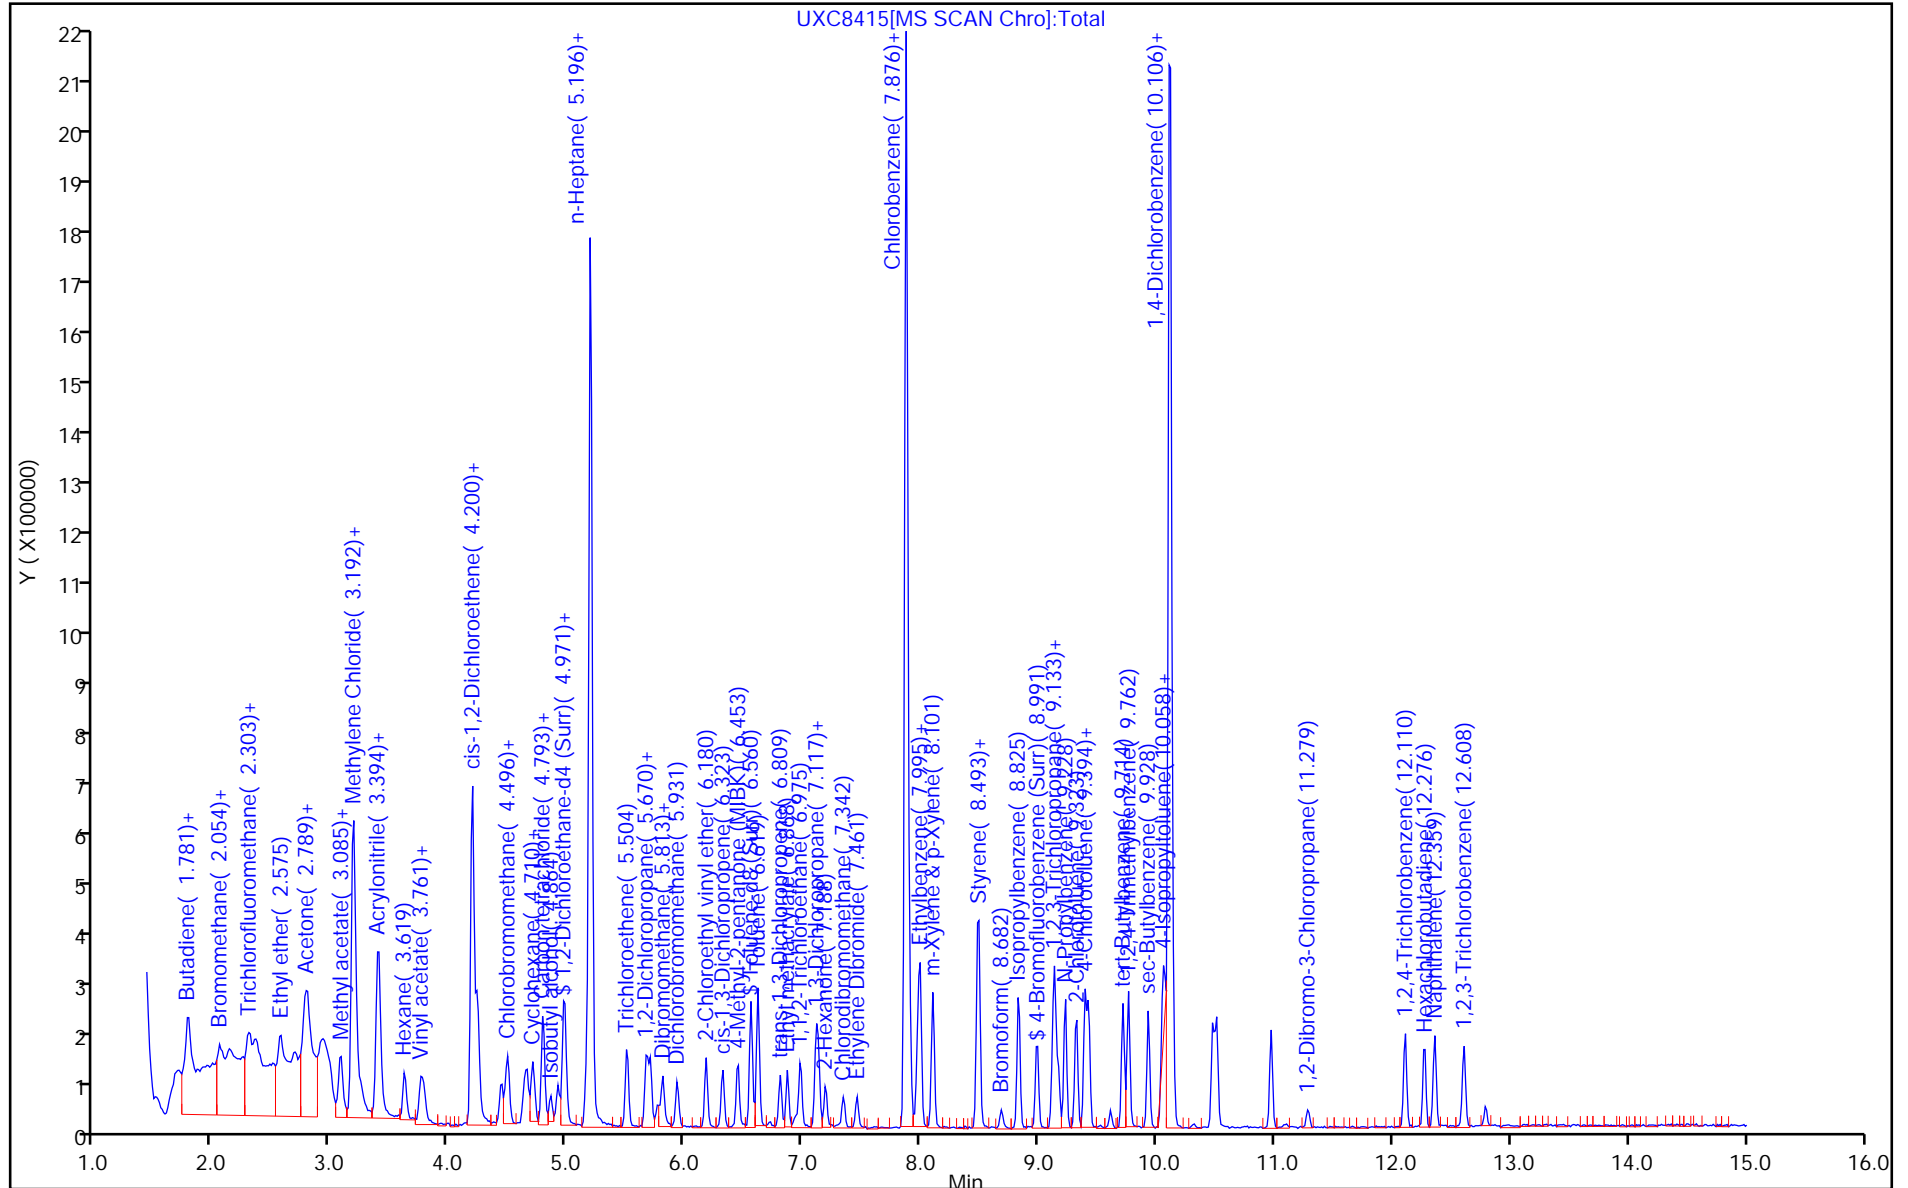

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8415.D
Injection Date: 21-Jan-2019 13:26:30 Instrument ID: A3UX15
Lims ID: STD8260 L1
Client ID:
Operator ID:
Purge Vol: 5.000 mL
Method: 8260_15
Column: DB-624 (0.18 mm)


ALS Bottle#: 6 Worklist Smp#: 7
Dil. Factor: 1.0000
Limit Group: MSV 8260B ICAL
Detector: MS SCAN

56 n-Heptane, CAS: 142-82-5

Signal: 1


Not Detected
Expected RT: 5.16

Processing Integration Results

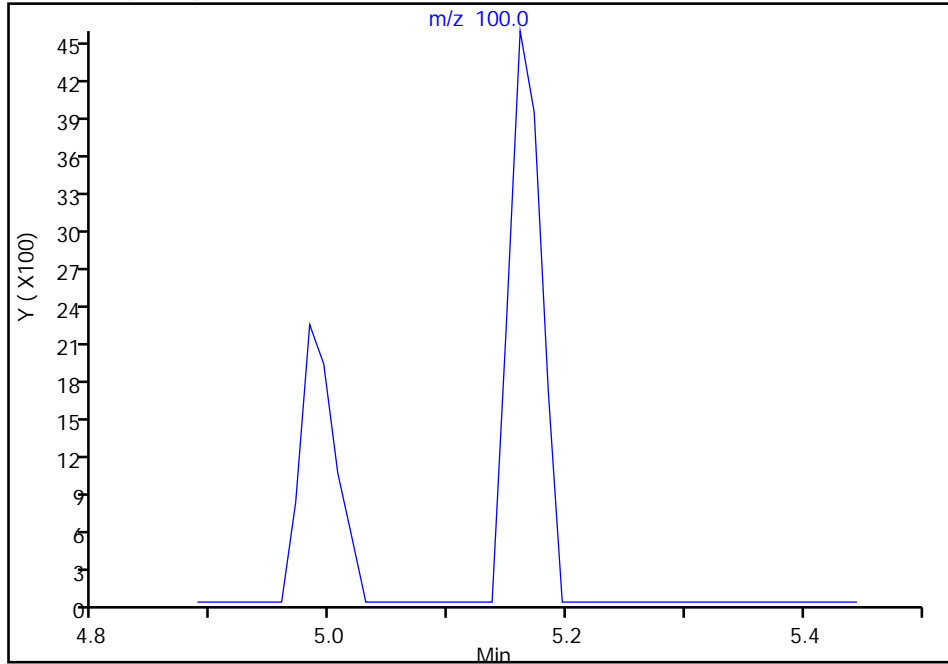

RT: 5.16
Area: 8801
Amount: 0.936957
Amount Units: ug/l

Manual Integration Results

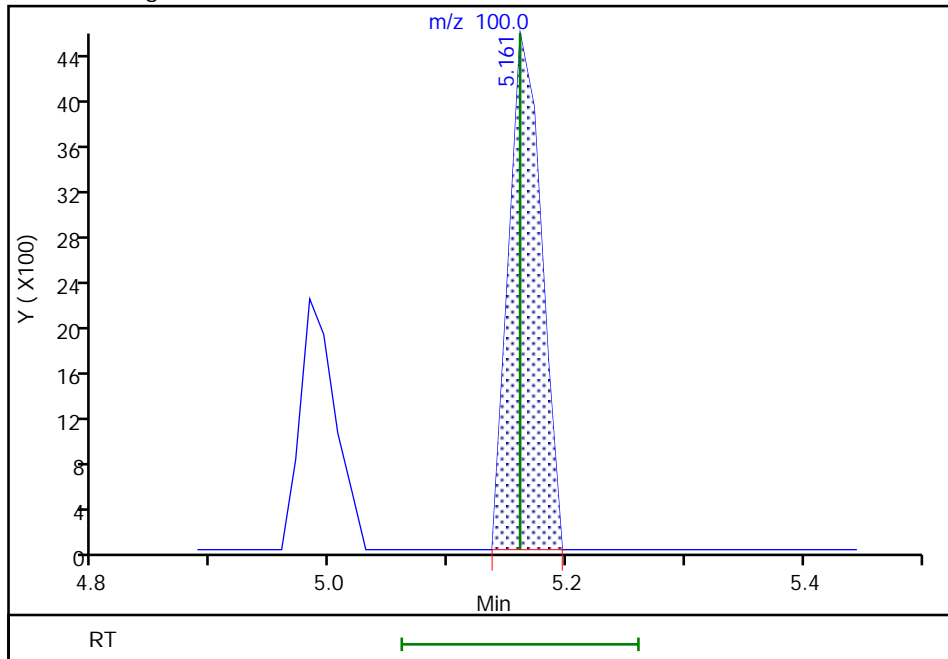

Reviewer: evansle, 21-Jan-2019 13:47:12
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

FORM I
GC/MS VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Client Sample ID: MW-131S_022619 Lab Sample ID: 240-108701-1
 Matrix: Water Lab File ID: UXC9107.D
 Analysis Method: 8260B Date Collected: 02/26/2019 09:47
 Sample wt/vol: 5 (mL) Date Analyzed: 03/01/2019 19:47
 Soil Aliquot Vol: _____ Dilution Factor: 1
 Soil Extract Vol.: _____ GC Column: DB-624 ID: 0.18 (mm)
 % Moisture: _____ Level: (low/med) Low
 Analysis Batch No.: 369935 Units: ug/L

CAS NO.	COMPOUND NAME	RESULT	Q	RL	MDL
75-35-4	1,1-Dichloroethene	1.0	U	1.0	0.19
156-59-2	cis-1,2-Dichloroethene	1.0	U	1.0	0.16
127-18-4	Tetrachloroethene	1.0	U	1.0	0.15
156-60-5	trans-1,2-Dichloroethene	1.0	U	1.0	0.19
79-01-6	Trichloroethene	1.0	U	1.0	0.10
75-01-4	Vinyl chloride	0.69	J	1.0	0.20

CAS NO.	SURROGATE	%REC	Q	LIMITS
17060-07-0	1,2-Dichloroethane-d4 (Surr)	93		70-121
460-00-4	4-Bromofluorobenzene (Surr)	67		59-120
2037-26-5	Toluene-d8 (Surr)	74		70-123
1868-53-7	Dibromofluoromethane (Surr)	94		75-128

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9107.D
 Lims ID: 240-108701-B-1
 Client ID: MW-131S_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 19:47:30 ALS Bottle#: 23 Worklist Smp#: 49
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-049
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

First Level Reviewer: evansle Date: 04-Mar-2019 08:13:42

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1359252	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1236329	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	92	708422	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	-0.001	95	242056	7.53	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	307948	7.45	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	890047	5.93	
\$ 7 4-Bromofluorobenzene (Surr	95	8.991	8.979	0.012	95	286392	5.34	
11 Vinyl chloride	62	1.781	1.781	0.000	95	27086	0.6908	
19 1,1-Dichloroethene	96		2.777				ND	
30 trans-1,2-Dichloroethene	96		3.405				ND	
39 cis-1,2-Dichloroethene	96		4.235				ND	
58 Trichloroethene	130		5.504				ND	
74 Tetrachloroethene	164		7.117				ND	

Reagents:

vm40ml_vials_00009 Amount Added: 0.00 Units: Run Reagent
 vm50ss_stk_00079 Amount Added: 0.80 Units: uL Run Reagent
 VM50IS_00072 Amount Added: 1.00 Units: uL Run Reagent
 vmDist_H2o_00139 Amount Added: 0.00 Units: Run Reagent

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9107.D

Injection Date: 01-Mar-2019 19:47:30

Instrument ID: A3UX15

Operator ID:

Lims ID: 240-108701-B-1

Lab Sample ID: 240-108701-1

Worklist Smp#: 49

Client ID: MW-131S_022619

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 23

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

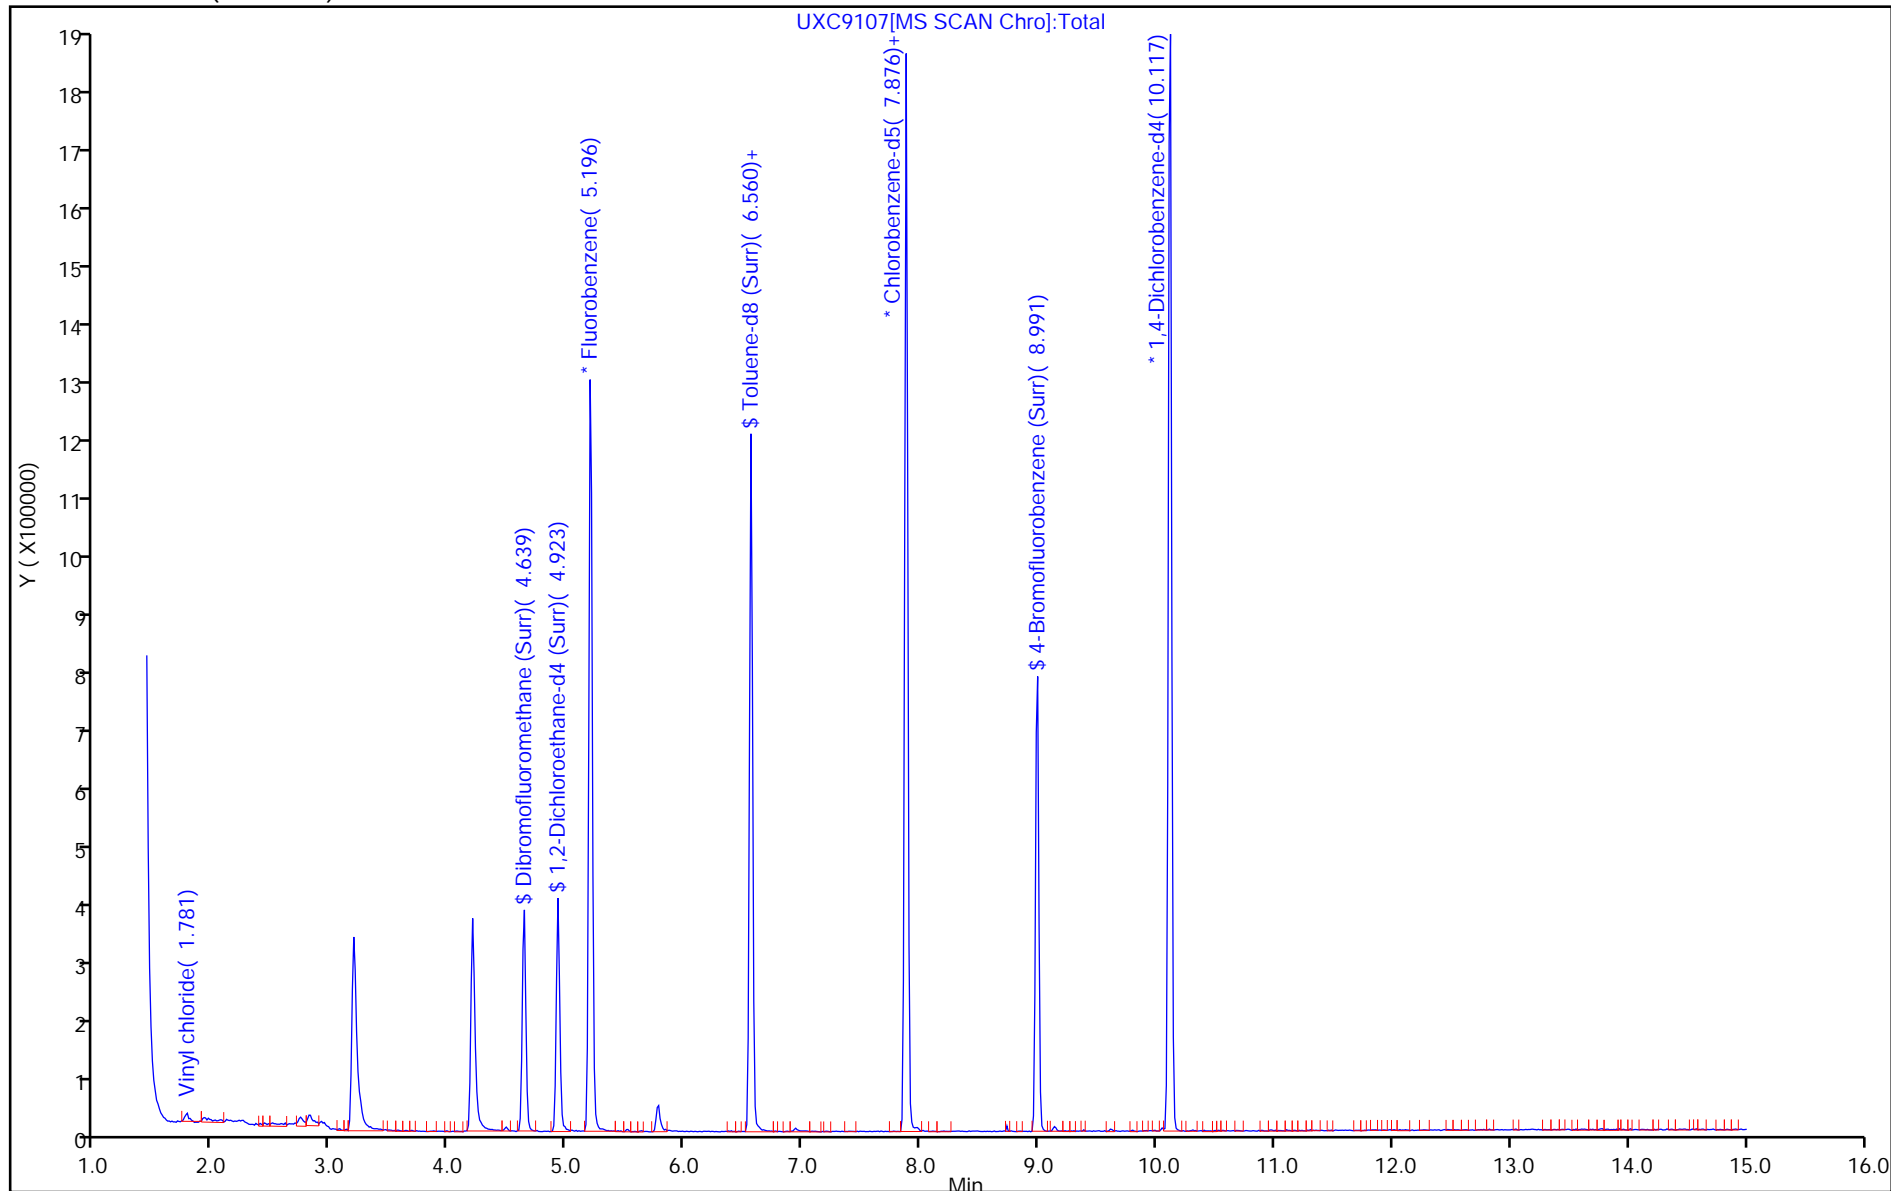

TestAmerica Canton
Recovery Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9107.D
 Lims ID: 240-108701-B-1
 Client ID: MW-131S_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 19:47:30 ALS Bottle#: 23 Worklist Smp#: 49
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-049
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

First Level Reviewer: evansle

Date: 04-Mar-2019 08:13:42

Compound	Amount Added	Amount Recovered	% Rec.
\$ 4 Dibromofluoromethane (Surr)	7.97	7.53	94.43
\$ 5 1,2-Dichloroethane-d4 (Surr)	7.97	7.45	93.45
\$ 6 Toluene-d8 (Surr)	7.97	5.93	74.42
\$ 7 4-Bromofluorobenzene (Surr)	7.97	5.34	66.95

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9107.D

Injection Date: 01-Mar-2019 19:47:30

Instrument ID: A3UX15

Lims ID: 240-108701-B-1

Lab Sample ID: 240-108701-1

Client ID: MW-131S_022619

Operator ID:

ALS Bottle#: 23 Worklist Smp#: 49

Purge Vol: 5.000 mL

Dil. Factor: 1.0000


Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

Detector: MS SCAN

11 Vinyl chloride, CAS: 75-01-4

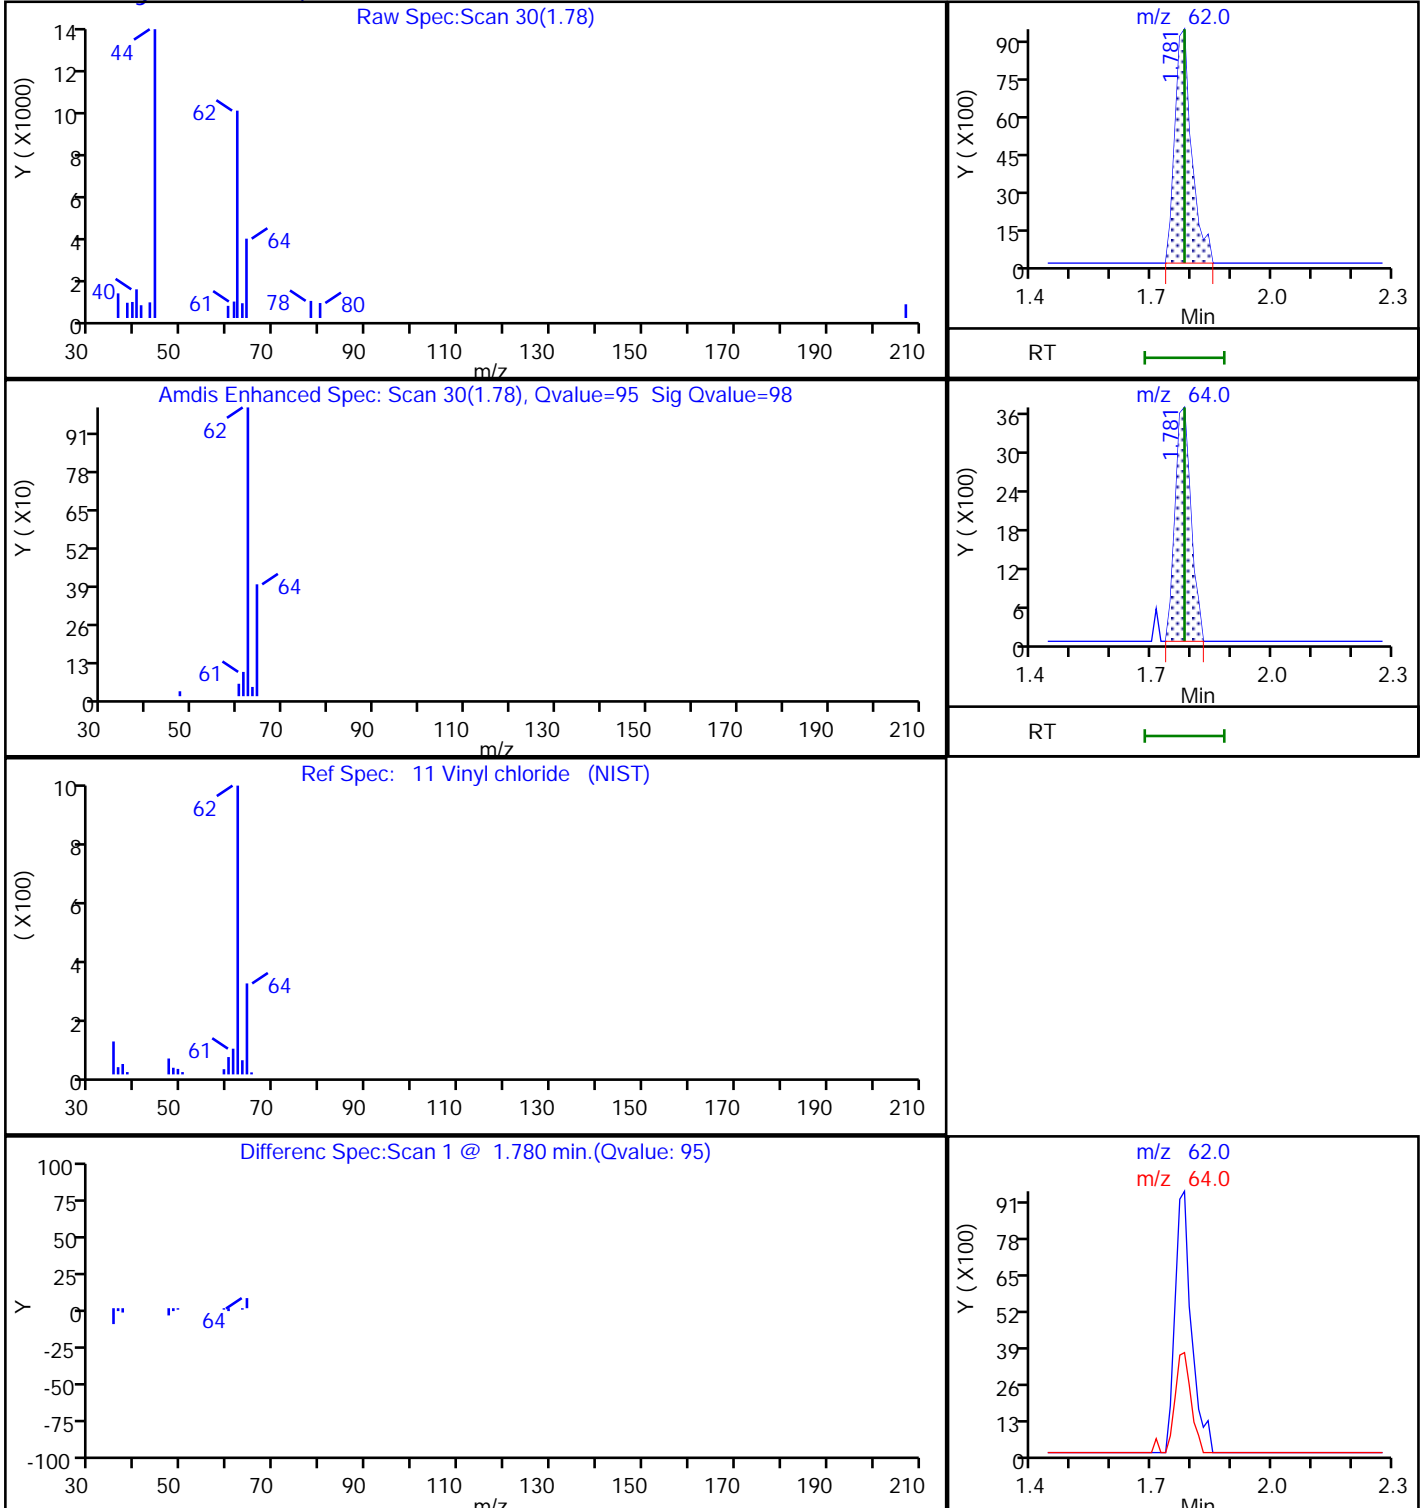

FORM I
GC/MS VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Client Sample ID: MW-132S_022619 Lab Sample ID: 240-108701-2
 Matrix: Water Lab File ID: UXC9108.D
 Analysis Method: 8260B Date Collected: 02/26/2019 11:22
 Sample wt/vol: 5(mL) Date Analyzed: 03/01/2019 20:09
 Soil Aliquot Vol: _____ Dilution Factor: 1
 Soil Extract Vol.: _____ GC Column: DB-624 ID: 0.18 (mm)
 % Moisture: _____ Level: (low/med) Low
 Analysis Batch No.: 369935 Units: ug/L

CAS NO.	COMPOUND NAME	RESULT	Q	RL	MDL
75-35-4	1,1-Dichloroethene	1.0	U	1.0	0.19
156-59-2	cis-1,2-Dichloroethene	1.0	U	1.0	0.16
127-18-4	Tetrachloroethene	1.0	U	1.0	0.15
156-60-5	trans-1,2-Dichloroethene	1.0	U	1.0	0.19
79-01-6	Trichloroethene	1.0	U	1.0	0.10
75-01-4	Vinyl chloride	1.0	U	1.0	0.20

CAS NO.	SURROGATE	%REC	Q	LIMITS
17060-07-0	1,2-Dichloroethane-d4 (Surr)	98		70-121
460-00-4	4-Bromofluorobenzene (Surr)	69		59-120
2037-26-5	Toluene-d8 (Surr)	76		70-123
1868-53-7	Dibromofluoromethane (Surr)	102		75-128

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9108.D
 Lims ID: 240-108701-B-2
 Client ID: MW-132S_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 20:09:30 ALS Bottle#: 24 Worklist Smp#: 50
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-050
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1027556	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	846842	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	528323	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	94	197557	8.13	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	243692	7.80	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	92	623445	6.07	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	94	202677	5.51	
11 Vinyl chloride	62		1.781				ND	
19 1,1-Dichloroethene	96		2.777				ND	
30 trans-1,2-Dichloroethene	96		3.405				ND	
39 cis-1,2-Dichloroethene	96		4.235				ND	
58 Trichloroethene	130		5.504				ND	
74 Tetrachloroethene	164		7.117				ND	

Reagents:

vm40ml_vials_00009 Amount Added: 0.00 Units: Run Reagent
 vm50ss_stk_00079 Amount Added: 0.80 Units: uL Run Reagent
 VM50IS_00072 Amount Added: 1.00 Units: uL Run Reagent
 vmDist_H2o_00139 Amount Added: 0.00 Units: Run Reagent

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9108.D

Injection Date: 01-Mar-2019 20:09:30

Instrument ID: A3UX15

Operator ID:

Lims ID: 240-108701-B-2

Lab Sample ID: 240-108701-2

Worklist Smp#: 50

Client ID: MW-132S_022619

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 24

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

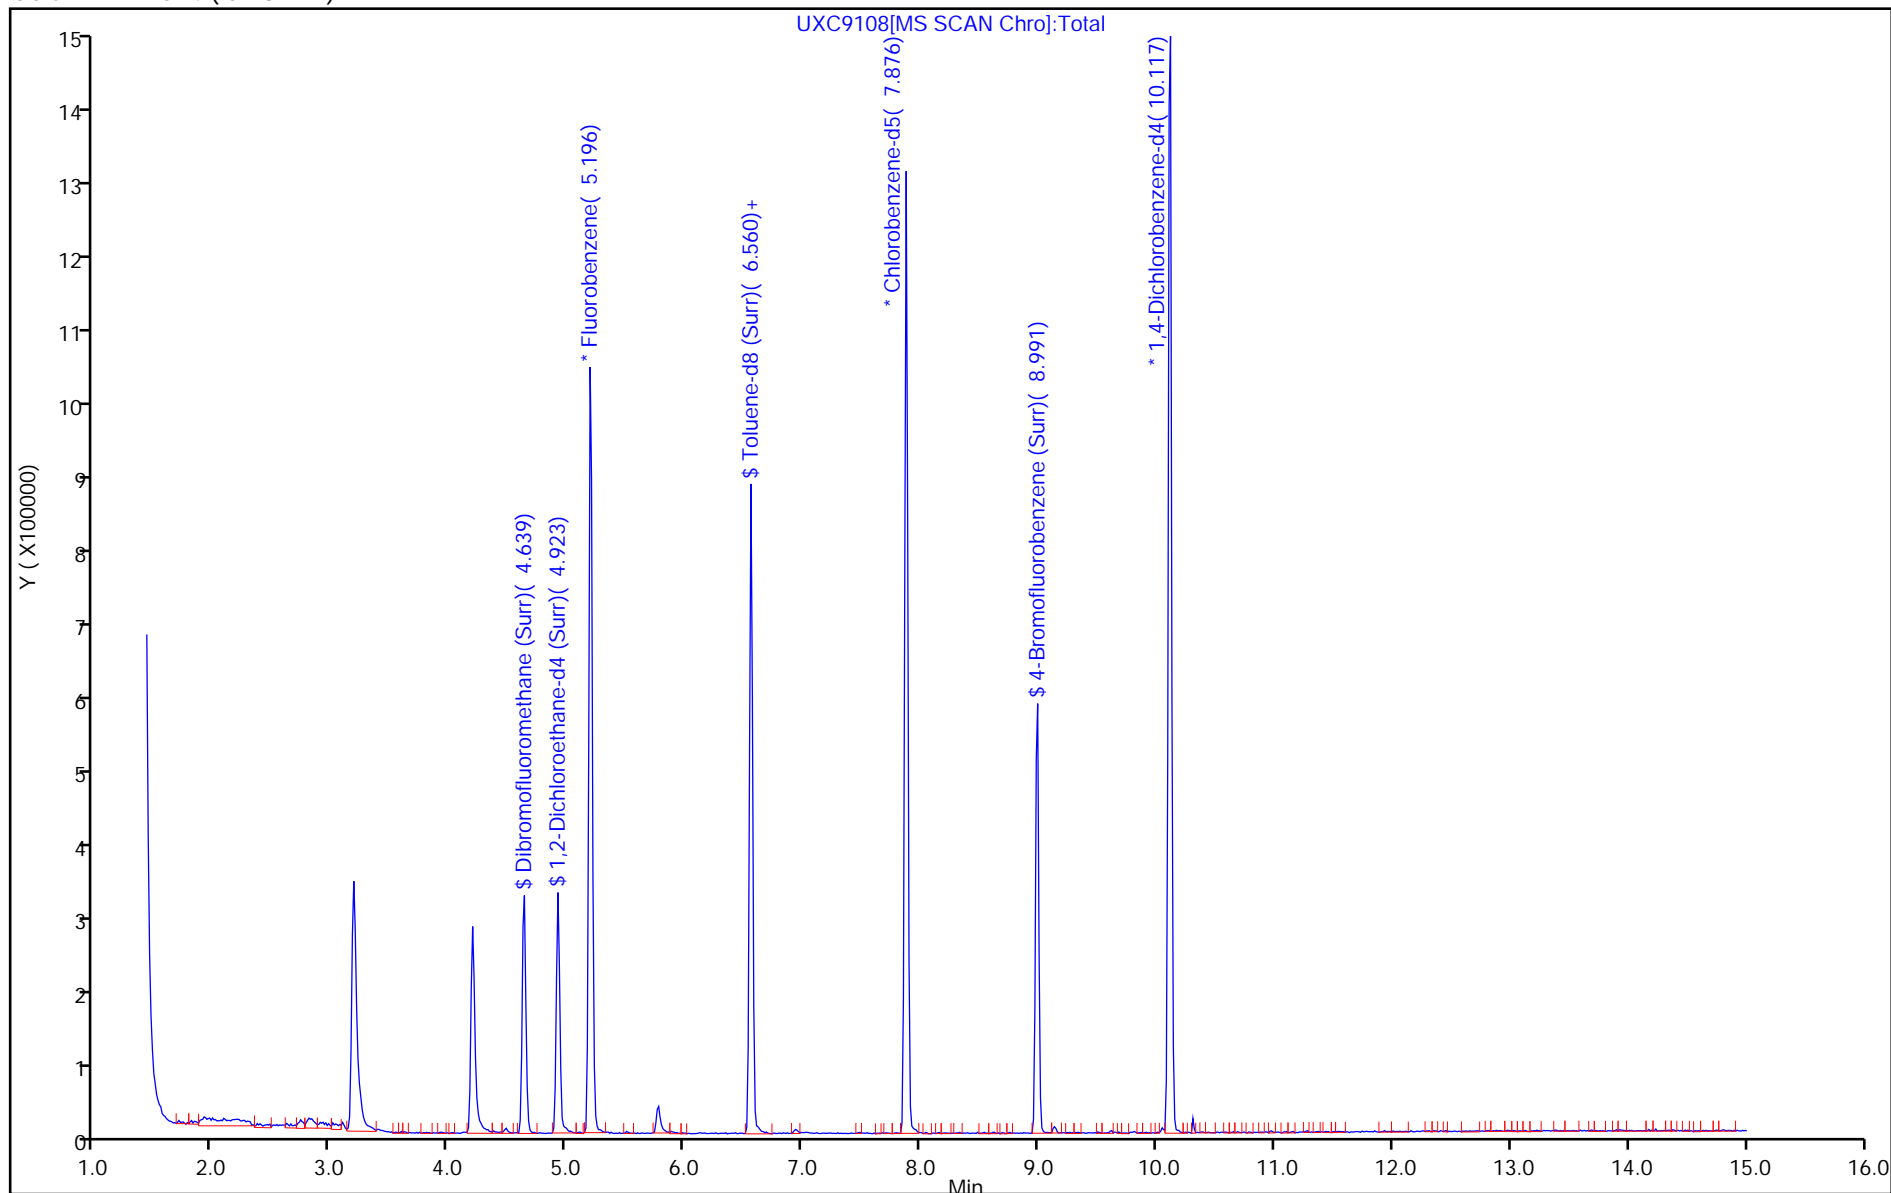

TestAmerica Canton
Recovery Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9108.D
 Lims ID: 240-108701-B-2
 Client ID: MW-132S_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 20:09:30 ALS Bottle#: 24 Worklist Smp#: 50
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-050
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Amount Added	Amount Recovered	% Rec.
\$ 4 Dibromofluoromethane (Surr)	7.97	8.13	101.95
\$ 5 1,2-Dichloroethane-d4 (Surr)	7.97	7.80	97.82
\$ 6 Toluene-d8 (Surr)	7.97	6.07	76.10
\$ 7 4-Bromofluorobenzene (Surr)	7.97	5.51	69.18

FORM I
GC/MS VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Client Sample ID: MW-85_022619 Lab Sample ID: 240-108701-3
 Matrix: Water Lab File ID: UXC9109.D
 Analysis Method: 8260B Date Collected: 02/26/2019 13:23
 Sample wt/vol: 5(mL) Date Analyzed: 03/01/2019 20:31
 Soil Aliquot Vol: _____ Dilution Factor: 1
 Soil Extract Vol.: _____ GC Column: DB-624 ID: 0.18 (mm)
 % Moisture: _____ Level: (low/med) Low
 Analysis Batch No.: 369935 Units: ug/L

CAS NO.	COMPOUND NAME	RESULT	Q	RL	MDL
75-35-4	1,1-Dichloroethene	1.0	U	1.0	0.19
156-59-2	cis-1,2-Dichloroethene	1.0	U	1.0	0.16
127-18-4	Tetrachloroethene	1.0	U	1.0	0.15
156-60-5	trans-1,2-Dichloroethene	1.0	U	1.0	0.19
79-01-6	Trichloroethene	1.0	U	1.0	0.10
75-01-4	Vinyl chloride	5.5		1.0	0.20

CAS NO.	SURROGATE	%REC	Q	LIMITS
17060-07-0	1,2-Dichloroethane-d4 (Surr)	93		70-121
460-00-4	4-Bromofluorobenzene (Surr)	65		59-120
2037-26-5	Toluene-d8 (Surr)	72		70-123
1868-53-7	Dibromofluoromethane (Surr)	91		75-128

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9109.D
 Lims ID: 240-108701-B-3
 Client ID: MW-85_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 20:31:30 ALS Bottle#: 25 Worklist Smp#: 51
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-051
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1366433	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1244445	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	728457	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	233556	7.22	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	307338	7.39	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	866335	5.74	
\$ 7 4-Bromofluorobenzene (Surr	95	8.979	8.979	0.000	95	279013	5.16	
11 Vinyl chloride	62	1.769	1.781	-0.012	98	215473	5.47	
19 1,1-Dichloroethene	96		2.777				ND	
30 trans-1,2-Dichloroethene	96		3.405				ND	
39 cis-1,2-Dichloroethene	96		4.235				ND	
58 Trichloroethene	130		5.504				ND	
74 Tetrachloroethene	164		7.117				ND	

Reagents:

vm40ml_vials_00009 Amount Added: 0.00 Units: Run Reagent
 vm50ss_stk_00079 Amount Added: 0.80 Units: uL Run Reagent
 VM50IS_00072 Amount Added: 1.00 Units: uL Run Reagent
 vmDist_H2o_00139 Amount Added: 0.00 Units: Run Reagent

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9109.D

Injection Date: 01-Mar-2019 20:31:30

Instrument ID: A3UX15

Operator ID:

Lims ID: 240-108701-B-3

Lab Sample ID: 240-108701-3

Worklist Smp#: 51

Client ID: MW-85_022619

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 25

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

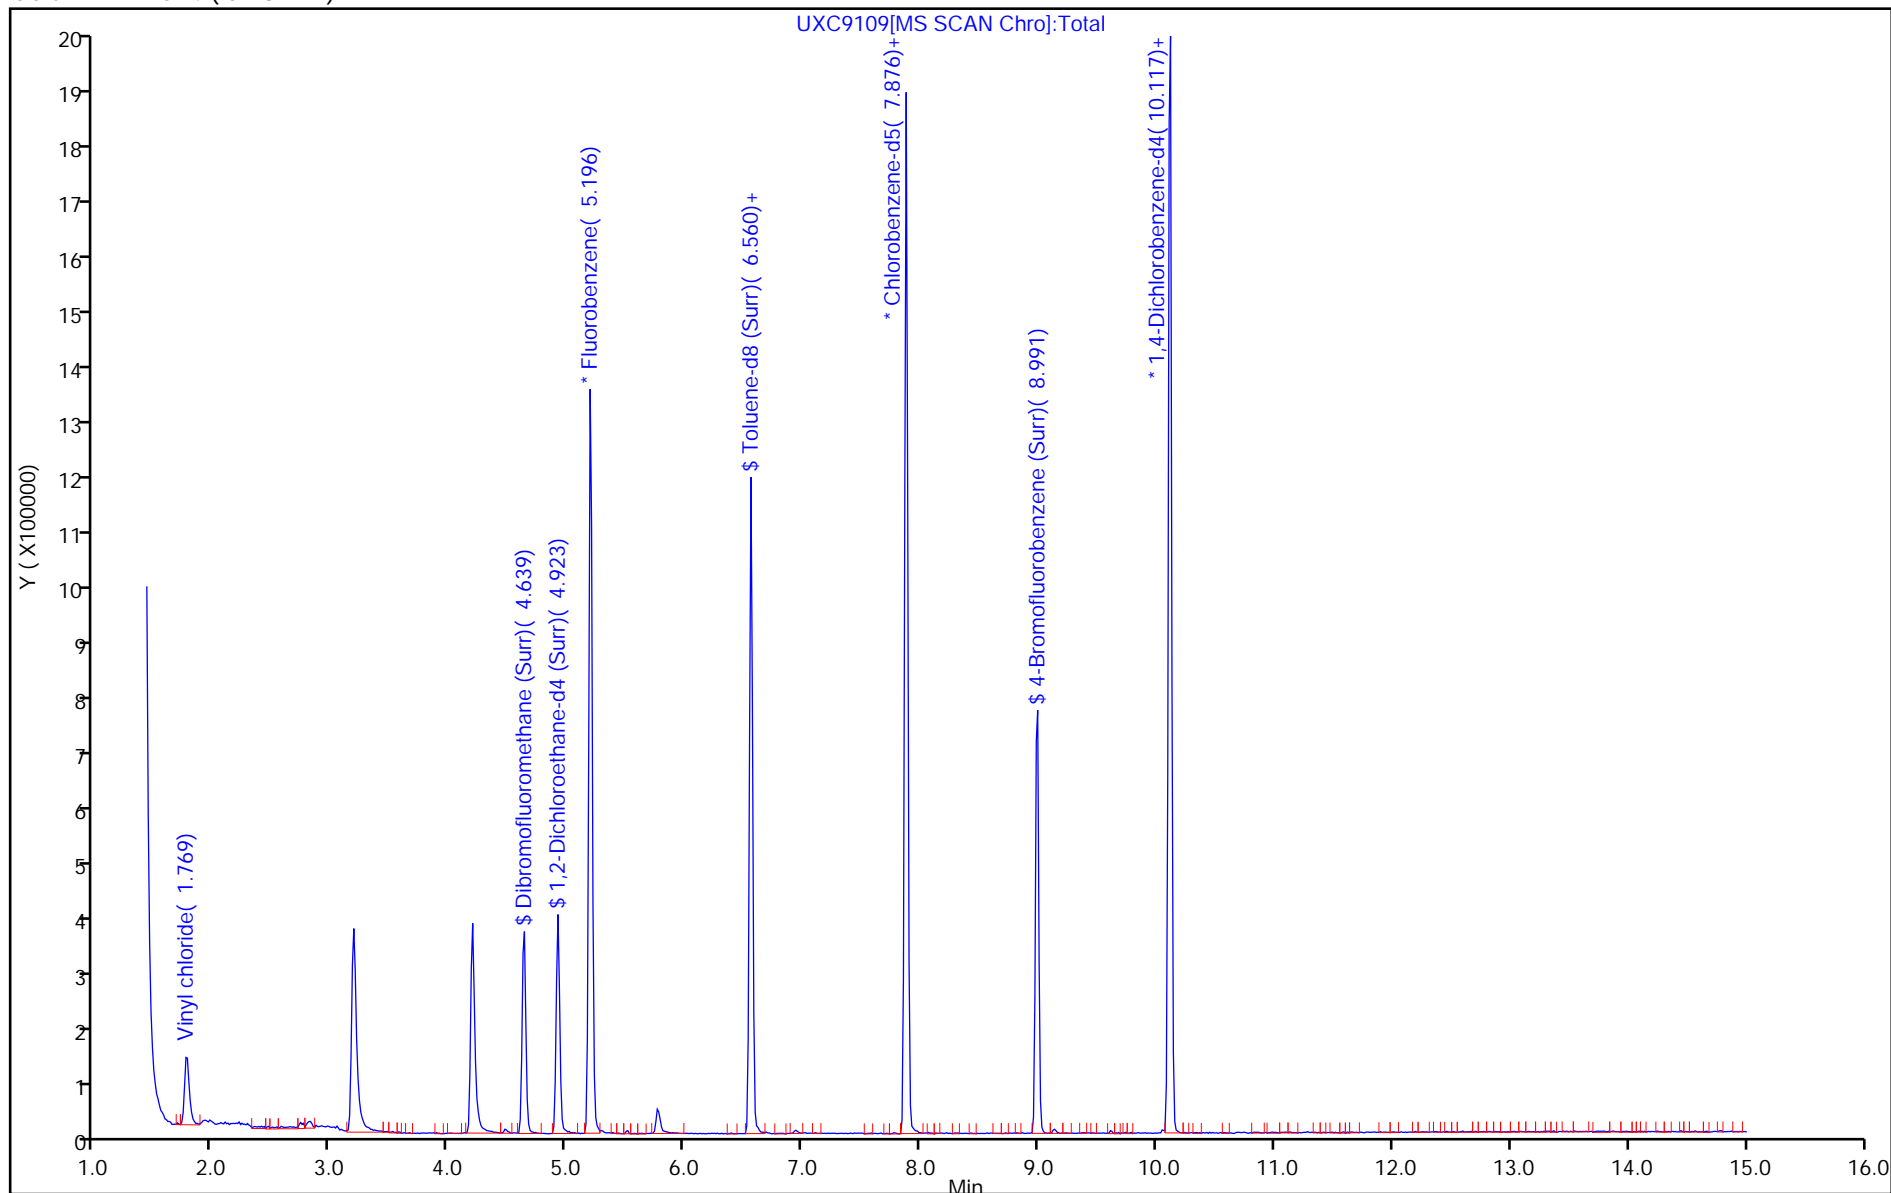

TestAmerica Canton
Recovery Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9109.D
 Lims ID: 240-108701-B-3
 Client ID: MW-85_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 20:31:30 ALS Bottle#: 25 Worklist Smp#: 51
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-051
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Amount Added	Amount Recovered	% Rec.
\$ 4 Dibromofluoromethane (Surr)	7.97	7.22	90.64
\$ 5 1,2-Dichloroethane-d4 (Surr)	7.97	7.39	92.78
\$ 6 Toluene-d8 (Surr)	7.97	5.74	71.96
\$ 7 4-Bromofluorobenzene (Surr)	7.97	5.16	64.80

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9109.D

Injection Date: 01-Mar-2019 20:31:30

Instrument ID: A3UX15

Lims ID: 240-108701-B-3

Lab Sample ID: 240-108701-3

Client ID: MW-85_022619

Operator ID:

ALS Bottle#: 25 Worklist Smp#: 51

Purge Vol: 5.000 mL

Dil. Factor: 1.0000


Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

Detector: MS SCAN

11 Vinyl chloride, CAS: 75-01-4

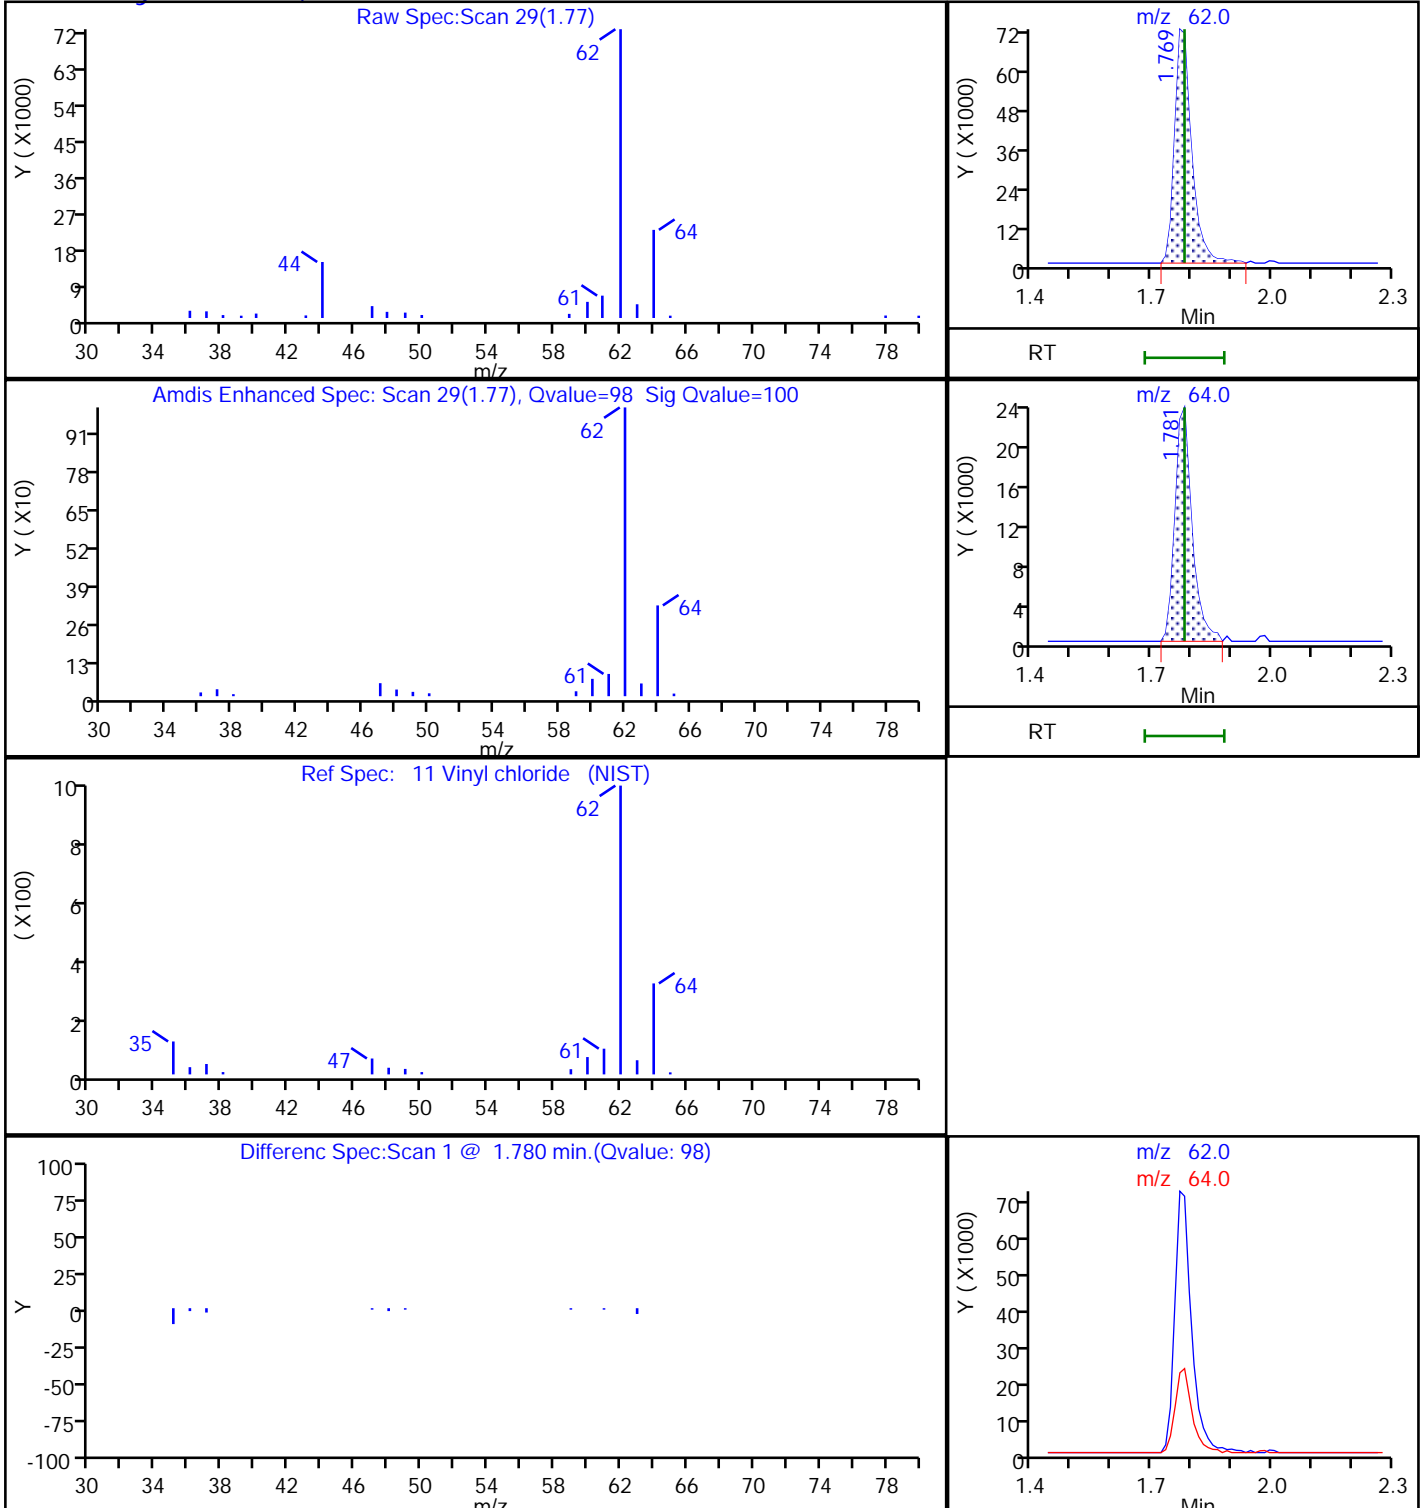

FORM I
GC/MS VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Client Sample ID: MW-78S_022619 Lab Sample ID: 240-108701-4
 Matrix: Water Lab File ID: UXC9110.D
 Analysis Method: 8260B Date Collected: 02/26/2019 15:47
 Sample wt/vol: 5(mL) Date Analyzed: 03/01/2019 20:53
 Soil Aliquot Vol: _____ Dilution Factor: 1
 Soil Extract Vol.: _____ GC Column: DB-624 ID: 0.18 (mm)
 % Moisture: _____ Level: (low/med) Low
 Analysis Batch No.: 369935 Units: ug/L

CAS NO.	COMPOUND NAME	RESULT	Q	RL	MDL
75-35-4	1,1-Dichloroethene	1.0	U	1.0	0.19
156-59-2	cis-1,2-Dichloroethene	1.0	U	1.0	0.16
127-18-4	Tetrachloroethene	1.0	U	1.0	0.15
156-60-5	trans-1,2-Dichloroethene	1.0	U	1.0	0.19
79-01-6	Trichloroethene	1.0	U	1.0	0.10
75-01-4	Vinyl chloride	1.0	U	1.0	0.20

CAS NO.	SURROGATE	%REC	Q	LIMITS
17060-07-0	1,2-Dichloroethane-d4 (Surr)	89		70-121
460-00-4	4-Bromofluorobenzene (Surr)	64		59-120
2037-26-5	Toluene-d8 (Surr)	72		70-123
1868-53-7	Dibromofluoromethane (Surr)	89		75-128

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9110.D
 Lims ID: 240-108701-B-4
 Client ID: MW-78S_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 20:53:30 ALS Bottle#: 26 Worklist Smp#: 52
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-052
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

First Level Reviewer: evansle

Date: 04-Mar-2019 08:14:16

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1395996	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	84	1289351	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	92	709168	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	233953	7.08	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	302394	7.12	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	895022	5.72	
\$ 7 4-Bromofluorobenzene (Surr	95	8.991	8.979	0.012	96	287162	5.13	
11 Vinyl chloride	62		1.781				ND	
19 1,1-Dichloroethene	96		2.777				ND	
30 trans-1,2-Dichloroethene	96		3.405				ND	
39 cis-1,2-Dichloroethene	96	4.236	4.235	0.001	79	4495	0.1046	
58 Trichloroethene	130		5.504				ND	
74 Tetrachloroethene	164		7.117				ND	

Reagents:

vm40ml_vials_00009	Amount Added: 0.00	Units:	Run Reagent
vm50ss_stk_00079	Amount Added: 0.80	Units: uL	Run Reagent
VM50IS_00072	Amount Added: 1.00	Units: uL	Run Reagent
vmDist_H2o_00139	Amount Added: 0.00	Units:	Run Reagent

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9110.D

Injection Date: 01-Mar-2019 20:53:30

Instrument ID: A3UX15

Operator ID:

Lims ID: 240-108701-B-4

Lab Sample ID: 240-108701-4

Worklist Smp#: 52

Client ID: MW-78S_022619

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 26

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

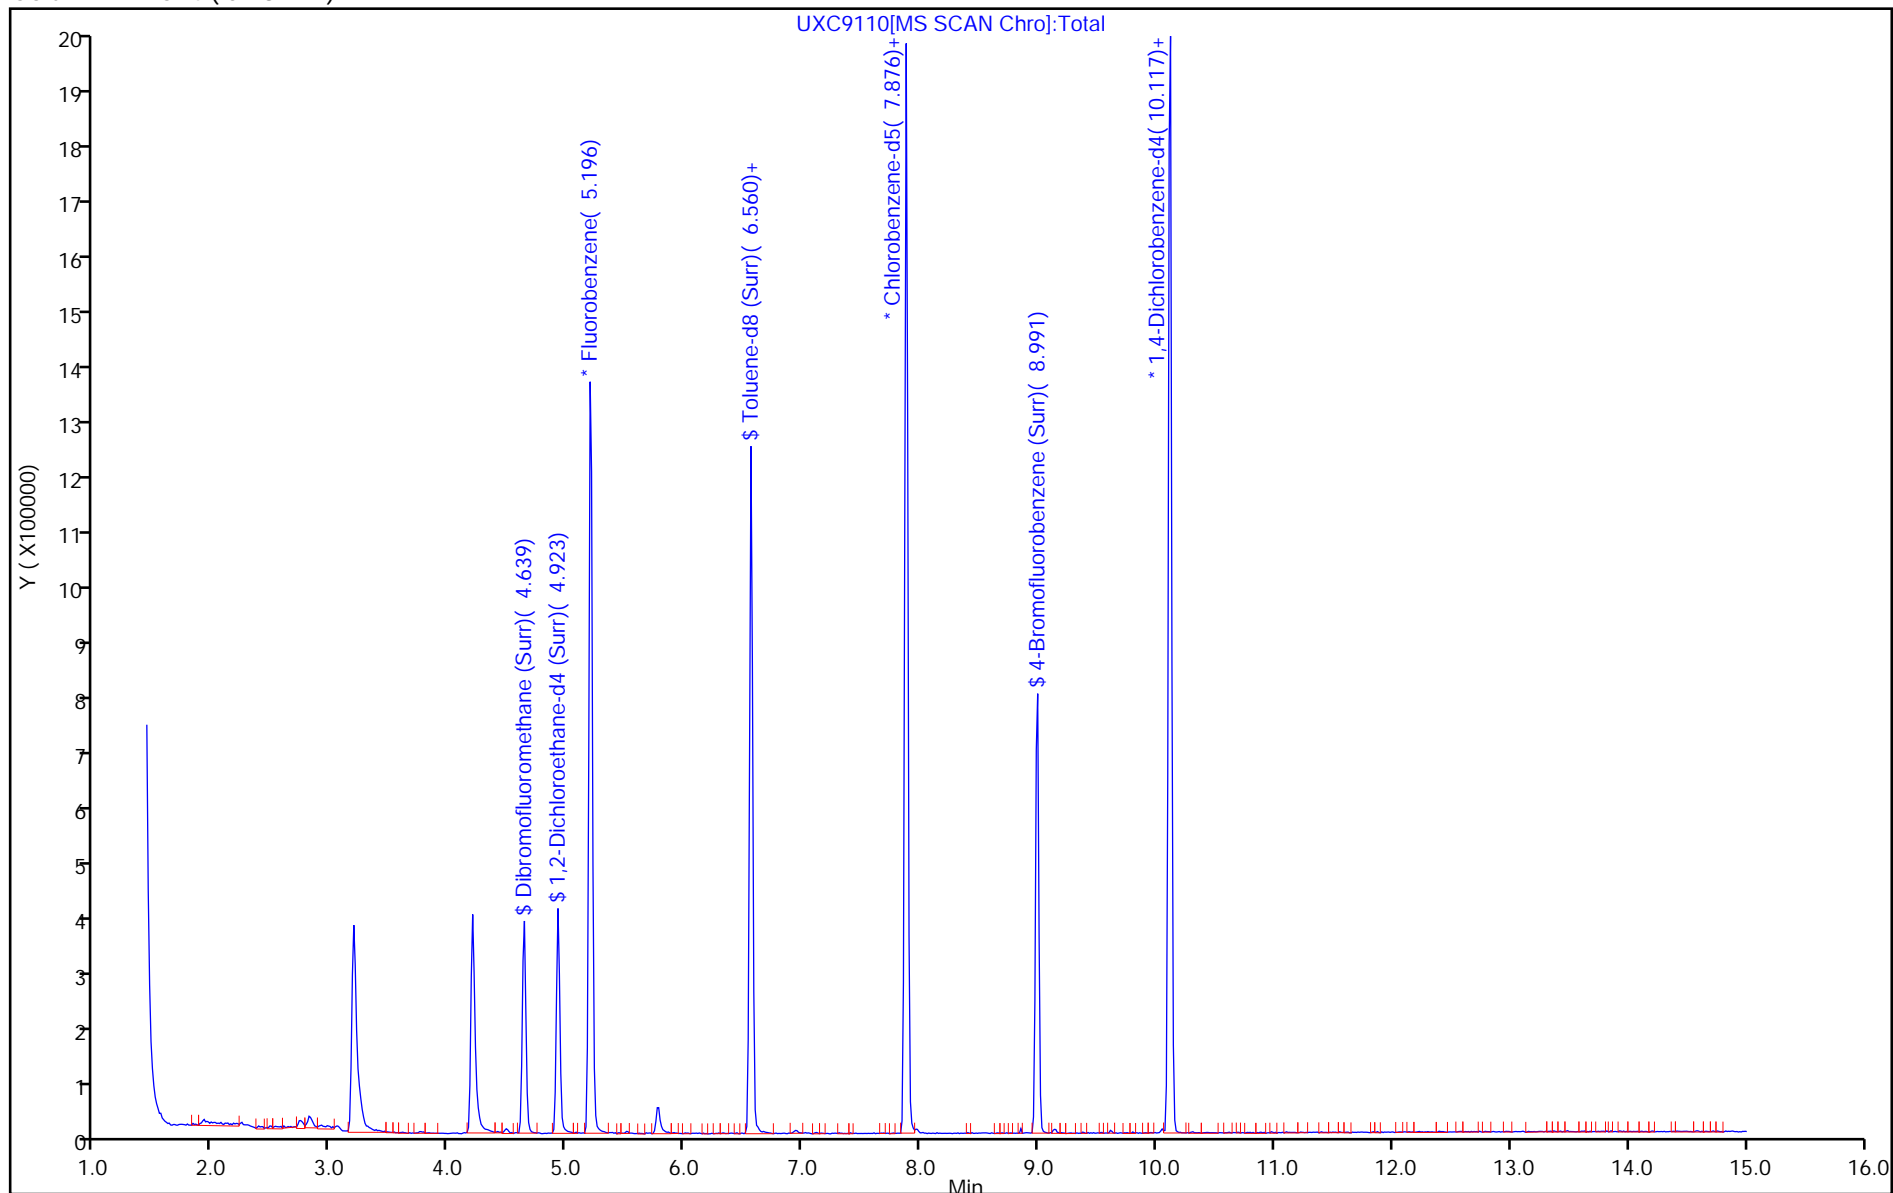

TestAmerica Canton
Recovery Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9110.D
 Lims ID: 240-108701-B-4
 Client ID: MW-78S_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 20:53:30 ALS Bottle#: 26 Worklist Smp#: 52
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-052
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: Deconvolution ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

First Level Reviewer: evansle

Date: 04-Mar-2019 08:14:16

Compound	Amount Added	Amount Recovered	% Rec.
\$ 4 Dibromofluoromethane (Surr)	7.97	7.08	88.87
\$ 5 1,2-Dichloroethane-d4 (Surr)	7.97	7.12	89.35
\$ 6 Toluene-d8 (Surr)	7.97	5.72	71.76
\$ 7 4-Bromofluorobenzene (Surr)	7.97	5.13	64.37

FORM I
GC/MS VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Client Sample ID: MW-78_022619 Lab Sample ID: 240-108701-5
 Matrix: Water Lab File ID: UXC9111.D
 Analysis Method: 8260B Date Collected: 02/26/2019 16:40
 Sample wt/vol: 5(mL) Date Analyzed: 03/01/2019 21:15
 Soil Aliquot Vol: _____ Dilution Factor: 1
 Soil Extract Vol.: _____ GC Column: DB-624 ID: 0.18 (mm)
 % Moisture: _____ Level: (low/med) Low
 Analysis Batch No.: 369935 Units: ug/L

CAS NO.	COMPOUND NAME	RESULT	Q	RL	MDL
75-35-4	1,1-Dichloroethene	1.0	U	1.0	0.19
156-59-2	cis-1,2-Dichloroethene	0.22	J	1.0	0.16
127-18-4	Tetrachloroethene	1.0	U	1.0	0.15
156-60-5	trans-1,2-Dichloroethene	1.0	U	1.0	0.19
79-01-6	Trichloroethene	1.0	U	1.0	0.10
75-01-4	Vinyl chloride	1.0	U	1.0	0.20

CAS NO.	SURROGATE	%REC	Q	LIMITS
17060-07-0	1,2-Dichloroethane-d4 (Surr)	98		70-121
460-00-4	4-Bromofluorobenzene (Surr)	68		59-120
2037-26-5	Toluene-d8 (Surr)	76		70-123
1868-53-7	Dibromofluoromethane (Surr)	101		75-128

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9111.D
 Lims ID: 240-108701-B-5
 Client ID: MW-78_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 21:15:30 ALS Bottle#: 27 Worklist Smp#: 53
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-053
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 09:22:51 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: RT Order ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	99	1097881	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	83	942373	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	93	567586	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	208155	8.01	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	100	261205	7.82	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	690561	6.04	
\$ 7 4-Bromofluorobenzene (Surr	95	8.991	8.979	0.012	96	222661	5.44	
11 Vinyl chloride	62		1.781				ND	
19 1,1-Dichloroethene	96		2.777				ND	
30 trans-1,2-Dichloroethene	96		3.405				ND	
39 cis-1,2-Dichloroethene	96	4.247	4.235	0.012	68	7394	0.2188	
58 Trichloroethene	130		5.504				ND	
74 Tetrachloroethene	164		7.117				ND	

Reagents:

vm40ml_vials_00009	Amount Added: 0.00	Units:	Run Reagent
vm50ss_stk_00079	Amount Added: 0.80	Units: uL	Run Reagent
VM50IS_00072	Amount Added: 1.00	Units: uL	Run Reagent
vmDist_H2o_00139	Amount Added: 0.00	Units:	Run Reagent

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9111.D

Injection Date: 01-Mar-2019 21:15:30

Instrument ID: A3UX15

Operator ID:

Lims ID: 240-108701-B-5

Lab Sample ID: 240-108701-5

Worklist Smp#: 53

Client ID: MW-78_022619

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 27

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

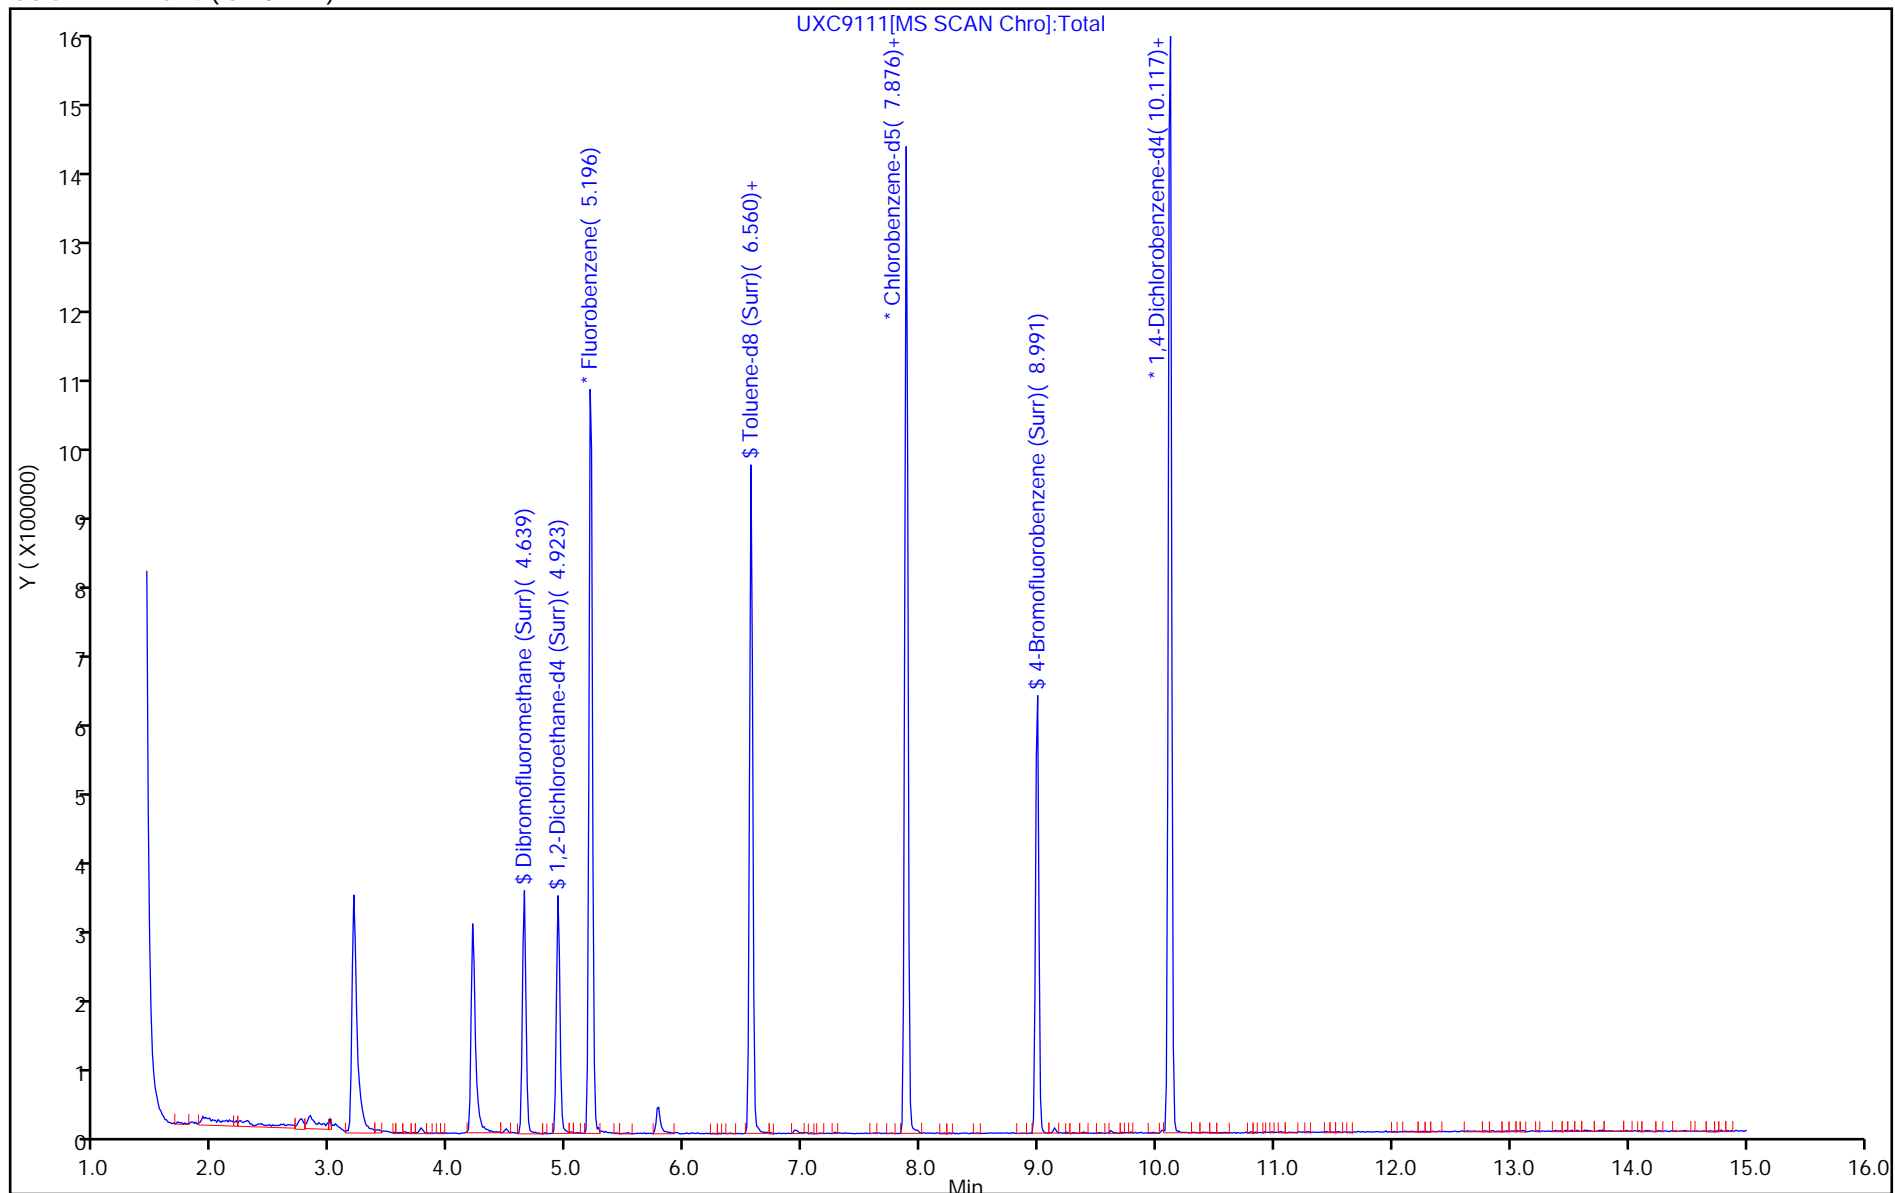

TestAmerica Canton
Recovery Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9111.D
 Lims ID: 240-108701-B-5
 Client ID: MW-78_022619
 Sample Type: Client
 Inject. Date: 01-Mar-2019 21:15:30 ALS Bottle#: 27 Worklist Smp#: 53
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-053
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 09:22:51 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: RT Order ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

Compound	Amount Added	Amount Recovered	% Rec.
\$ 4 Dibromofluoromethane (Surr)	7.97	8.01	100.54
\$ 5 1,2-Dichloroethane-d4 (Surr)	7.97	7.82	98.14
\$ 6 Toluene-d8 (Surr)	7.97	6.04	75.75
\$ 7 4-Bromofluorobenzene (Surr)	7.97	5.44	68.29

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9111.D

Injection Date: 01-Mar-2019 21:15:30

Instrument ID: A3UX15

Lims ID: 240-108701-B-5

Lab Sample ID: 240-108701-5

Client ID: MW-78_022619

Operator ID:

ALS Bottle#: 27

Worklist Smp#: 53

Purge Vol: 5.000 mL

Dil. Factor: 1.0000


Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

Detector: MS SCAN

39 cis-1,2-Dichloroethene, CAS: 156-59-2

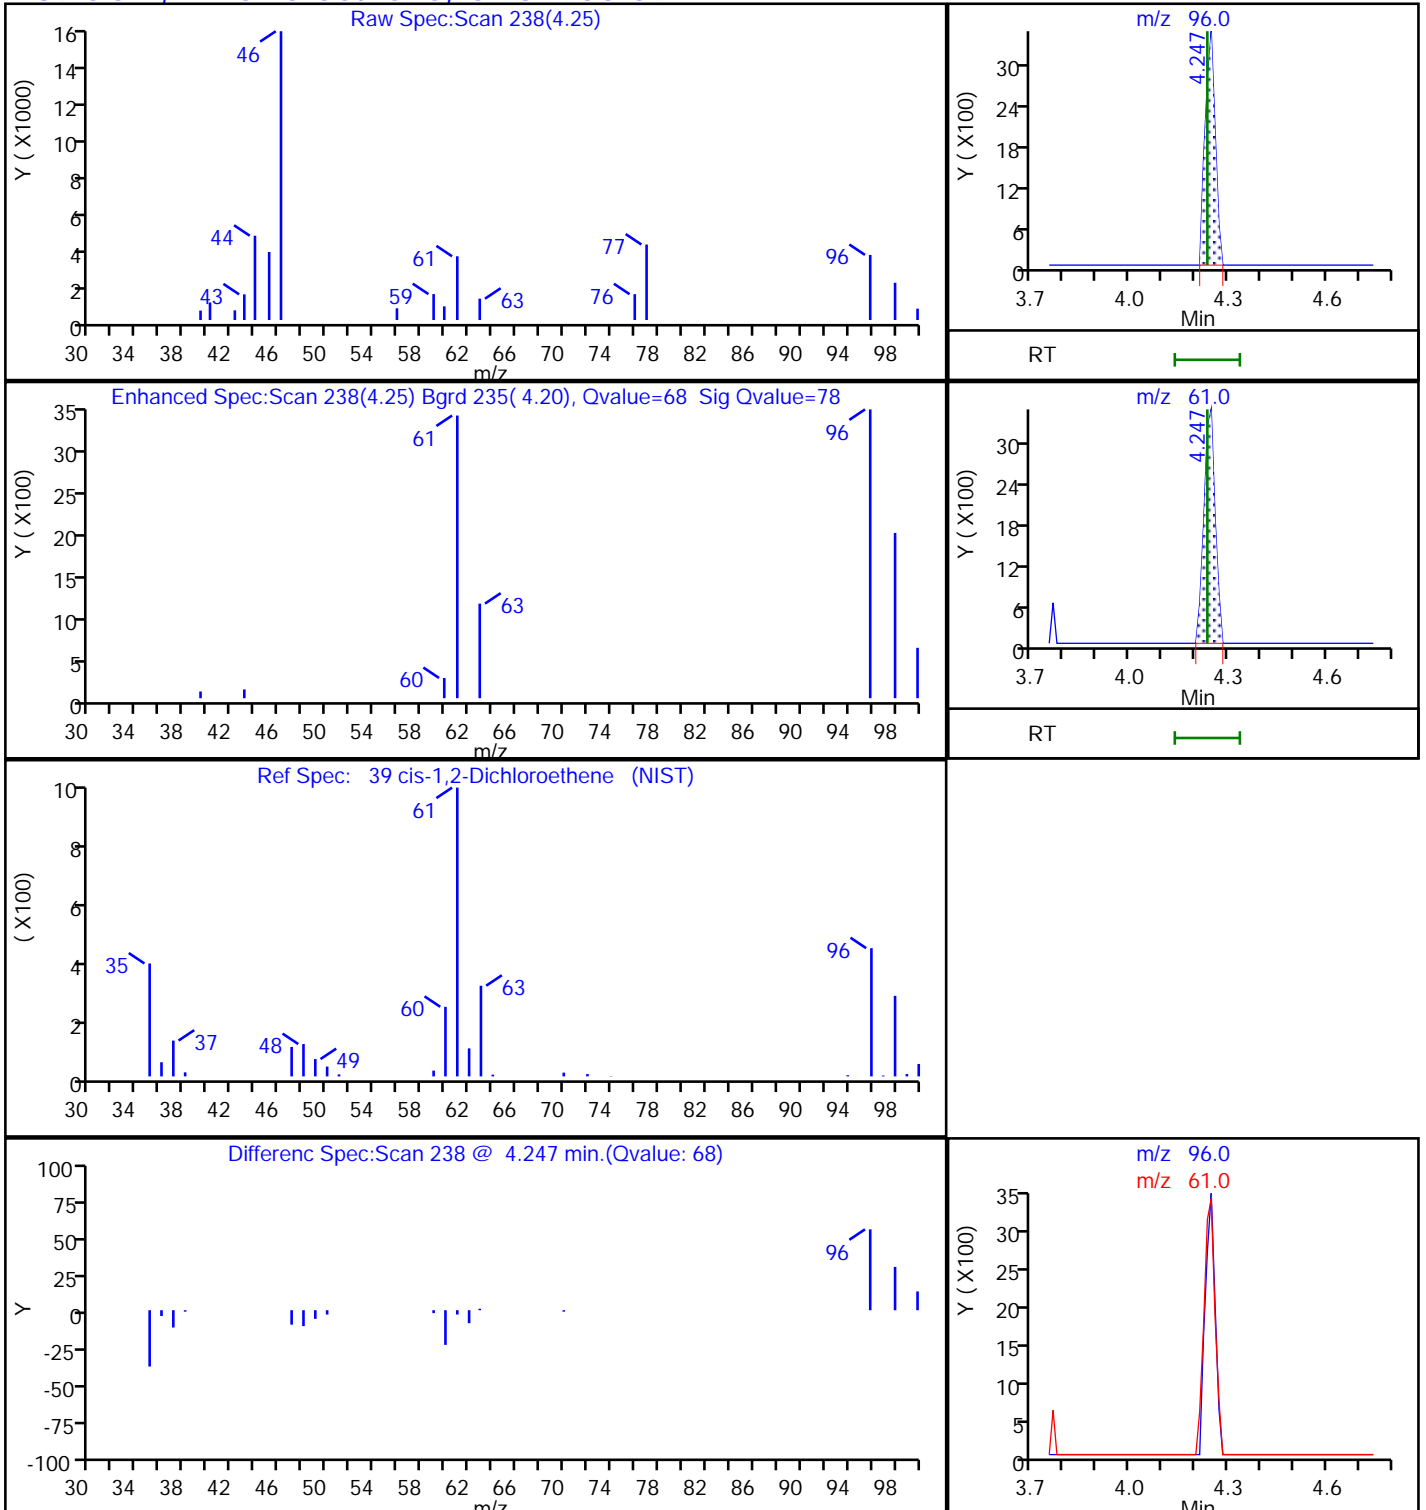

FORM I
GC/MS VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Canton Job No.: 240-108701-1
 SDG No.: _____
 Client Sample ID: TRIP BLANK Lab Sample ID: 240-108701-6
 Matrix: Water Lab File ID: UXC9112.D
 Analysis Method: 8260B Date Collected: 02/26/2019 00:00
 Sample wt/vol: 5 (mL) Date Analyzed: 03/01/2019 21:37
 Soil Aliquot Vol: _____ Dilution Factor: 1
 Soil Extract Vol.: _____ GC Column: DB-624 ID: 0.18 (mm)
 % Moisture: _____ Level: (low/med) Low
 Analysis Batch No.: 369935 Units: ug/L

CAS NO.	COMPOUND NAME	RESULT	Q	RL	MDL
75-35-4	1,1-Dichloroethene	1.0	U	1.0	0.19
156-59-2	cis-1,2-Dichloroethene	1.0	U	1.0	0.16
127-18-4	Tetrachloroethene	1.0	U	1.0	0.15
156-60-5	trans-1,2-Dichloroethene	1.0	U	1.0	0.19
79-01-6	Trichloroethene	1.0	U	1.0	0.10
75-01-4	Vinyl chloride	1.0	U	1.0	0.20

CAS NO.	SURROGATE	%REC	Q	LIMITS
17060-07-0	1,2-Dichloroethane-d4 (Surr)	101		70-121
460-00-4	4-Bromofluorobenzene (Surr)	71		59-120
2037-26-5	Toluene-d8 (Surr)	78		70-123
1868-53-7	Dibromofluoromethane (Surr)	103		75-128

TestAmerica Canton
Target Compound Quantitation Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9112.D
 Lims ID: 240-108701-A-6
 Client ID: TRIP BLANK
 Sample Type: Client
 Inject. Date: 01-Mar-2019 21:37:30 ALS Bottle#: 28 Worklist Smp#: 54
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-054
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: RT Order ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

First Level Reviewer: evansle Date: 04-Mar-2019 08:17:00

Compound	Sig	RT (min.)	Exp RT (min.)	Dlt RT (min.)	Q	Response	OnCol Amt ug/l	Flags
* 1 Fluorobenzene	96	5.196	5.196	0.000	100	1242595	10.0	
* 2 Chlorobenzene-d5	117	7.876	7.876	0.000	83	1125353	10.0	
* 3 1,4-Dichlorobenzene-d4	152	10.117	10.117	0.000	92	641240	10.0	
\$ 4 Dibromofluoromethane (Surr	113	4.639	4.639	0.000	95	240407	8.18	
\$ 5 1,2-Dichloroethane-d4 (Sur	65	4.923	4.923	0.000	99	303000	8.02	
\$ 6 Toluene-d8 (Surr)	98	6.560	6.560	0.000	93	851699	6.24	
\$ 7 4-Bromofluorobenzene (Surr	95	8.991	8.979	0.012	96	276929	5.67	
11 Vinyl chloride	62		1.781				ND	
19 1,1-Dichloroethene	96		2.777				ND	
30 trans-1,2-Dichloroethene	96		3.405				ND	
39 cis-1,2-Dichloroethene	96		4.235				ND	
58 Trichloroethene	130		5.504				ND	
74 Tetrachloroethene	164		7.117				ND	

Reagents:

vm40ml_vials_00009 Amount Added: 0.00 Units: Run Reagent
 vm50ss_stk_00079 Amount Added: 0.80 Units: uL Run Reagent
 VM50IS_00072 Amount Added: 1.00 Units: uL Run Reagent
 vmDist_H2o_00139 Amount Added: 0.00 Units: Run Reagent

TestAmerica Canton

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9112.D

Injection Date: 01-Mar-2019 21:37:30

Instrument ID: A3UX15

Operator ID:

Lims ID: 240-108701-A-6

Lab Sample ID: 240-108701-6

Worklist Smp#: 54

Client ID: TRIP BLANK

Purge Vol: 5.000 mL


Dil. Factor: 1.0000

ALS Bottle#: 28

Method: 8260_15

Limit Group: MSV 8260B ICAL

Column: DB-624 (0.18 mm)

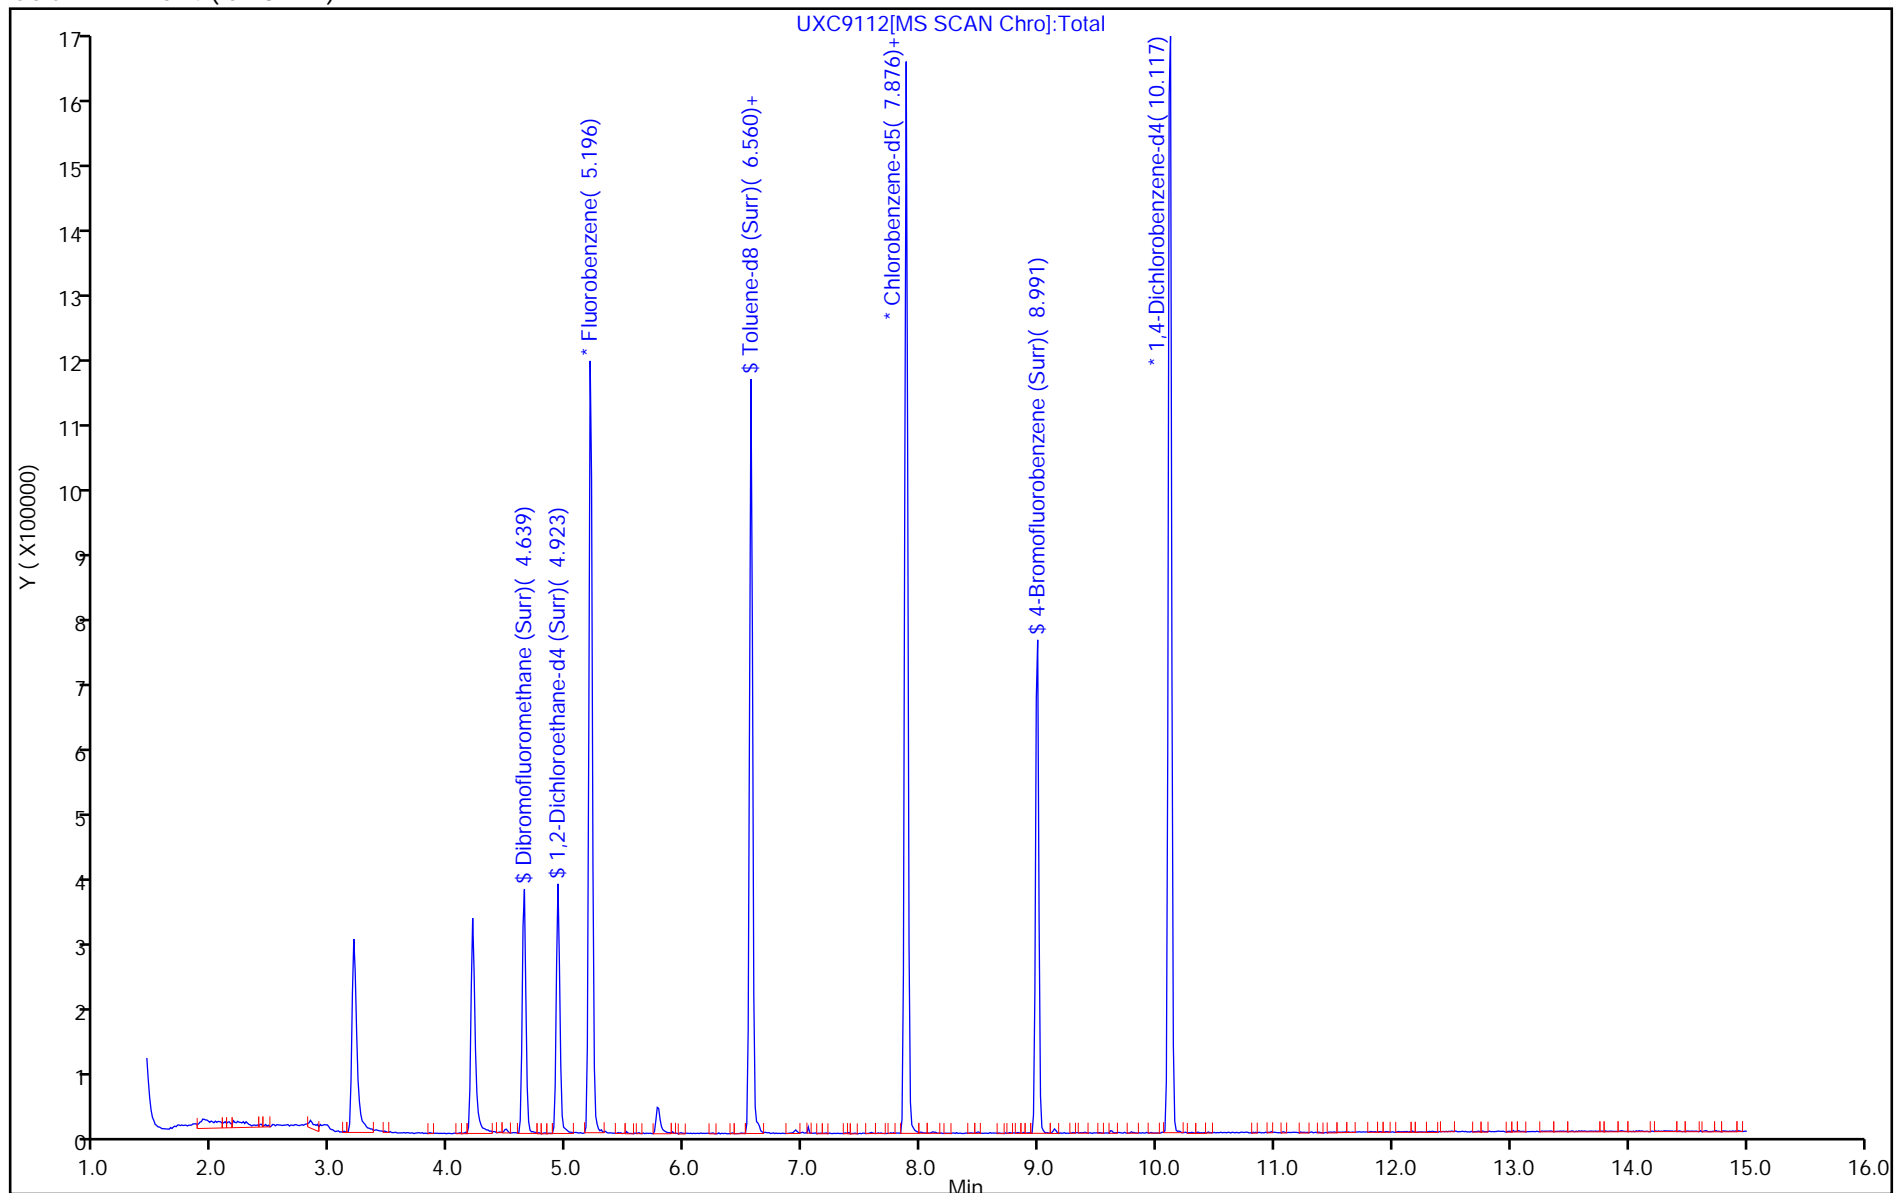

TestAmerica Canton
Recovery Report

Data File: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\UXC9112.D
 Lims ID: 240-108701-A-6
 Client ID: TRIP BLANK
 Sample Type: Client
 Inject. Date: 01-Mar-2019 21:37:30 ALS Bottle#: 28 Worklist Smp#: 54
 Purge Vol: 5.000 mL Dil. Factor: 1.0000
 Sample Info: 240-0084835-054
 Misc. Info.: C90301A,8260LLUX15,,43582
 Operator ID: Instrument ID: A3UX15
 Method: \\chromna\Canton\ChromData\A3UX15\20190301-84835.b\8260_15.m
 Limit Group: MSV 8260B ICAL
 Last Update: 04-Mar-2019 08:15:15 Calib Date: 21-Jan-2019 19:15:30
 Integrator: RTE ID Type: RT Order ID
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromna\Canton\ChromData\A3UX15\20190121-83824.b\UXC8431.D
 Column 1 : DB-624 (0.18 mm) Det: MS SCAN
 Process Host: CTX0306

First Level Reviewer: evansle Date: 04-Mar-2019 08:17:00

Compound	Amount Added	Amount Recovered	% Rec.
\$ 4 Dibromofluoromethane (Surr)	7.97	8.18	102.59
\$ 5 1,2-Dichloroethane-d4 (Surr)	7.97	8.02	100.58
\$ 6 Toluene-d8 (Surr)	7.97	6.24	78.24
\$ 7 4-Bromofluorobenzene (Surr)	7.97	5.67	71.13

Surrogate Summary

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Matrix: Water

Prep Type: Total/NA

Percent Surrogate Recovery (Acceptance Limits)

Lab Sample ID	Client Sample ID	Percent Surrogate Recovery (Acceptance Limits)			
		DCA (70-121)	BFB (59-120)	TOL (70-123)	DBFM (75-128)
240-108594-E-3 MS	Matrix Spike	91	80	81	101
240-108594-H-3 MSD	Matrix Spike Duplicate	89	81	81	99
240-108701-1	MW-131S_022619	93	67	74	94
240-108701-2	MW-132S_022619	98	69	76	102
240-108701-3	MW-85_022619	93	65	72	91
240-108701-4	MW-78S_022619	89	64	72	89
240-108701-5	MW-78_022619	98	68	76	101
240-108701-6	TRIP BLANK	101	71	78	103
LCS 240-369935/4	Lab Control Sample	92	84	86	101
MB 240-369935/6	Method Blank	90	70	75	93

Surrogate Legend

DCA = 1,2-Dichloroethane-d4 (Surr)

BFB = 4-Bromofluorobenzene (Surr)

TOL = Toluene-d8 (Surr)

DBFM = Dibromofluoromethane (Surr)

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Matrix: Water

Prep Type: Total/NA

Percent Surrogate Recovery (Acceptance Limits)

Lab Sample ID	Client Sample ID	DCA
		(63-125)
240-108589-B-1 MS	Matrix Spike	82
240-108589-B-1 MSD	Matrix Spike Duplicate	82
240-108701-1	MW-131S_022619	85
240-108701-2	MW-132S_022619	82
240-108701-3	MW-85_022619	81
240-108701-4	MW-78S_022619	81
240-108701-5	MW-78_022619	82
LCS 240-370005/4	Lab Control Sample	84
MB 240-370005/5	Method Blank	80

Surrogate Legend

DCA = 1,2-Dichloroethane-d4 (Surr)

QC Sample Results

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Method: 8260B - Volatile Organic Compounds (GC/MS)

Lab Sample ID: MB 240-369935/6

Matrix: Water

Analysis Batch: 369935

Client Sample ID: Method Blank

Prep Type: Total/NA

Analyte	MB Result	MB Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,1-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 13:00	1
cis-1,2-Dichloroethene	1.0	U	1.0	0.16	ug/L			03/01/19 13:00	1
Tetrachloroethene	1.0	U	1.0	0.15	ug/L			03/01/19 13:00	1
trans-1,2-Dichloroethene	1.0	U	1.0	0.19	ug/L			03/01/19 13:00	1
Trichloroethene	1.0	U	1.0	0.10	ug/L			03/01/19 13:00	1
Vinyl chloride	1.0	U	1.0	0.20	ug/L			03/01/19 13:00	1

Surrogate	MB %Recovery	MB Qualifier	Limits	Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	90		70 - 121		03/01/19 13:00	1
4-Bromofluorobenzene (Surr)	70		59 - 120		03/01/19 13:00	1
Toluene-d8 (Surr)	75		70 - 123		03/01/19 13:00	1
Dibromofluoromethane (Surr)	93		75 - 128		03/01/19 13:00	1

Lab Sample ID: LCS 240-369935/4

Matrix: Water

Analysis Batch: 369935

Client Sample ID: Lab Control Sample

Prep Type: Total/NA

Analyte	Spike Added	LCS Result	LCS Qualifier	Unit	D	%Rec	%Rec. Limits
1,1-Dichloroethene	10.0	10.7		ug/L		107	65 - 139
cis-1,2-Dichloroethene	10.0	12.4		ug/L		124	76 - 128
Tetrachloroethene	10.0	11.6		ug/L		116	74 - 130
trans-1,2-Dichloroethene	10.0	12.9		ug/L		129	78 - 133
Trichloroethene	10.0	12.2		ug/L		122	76 - 125
Vinyl chloride	10.0	10.5		ug/L		105	58 - 143

Surrogate	LCS %Recovery	LCS Qualifier	Limits
1,2-Dichloroethane-d4 (Surr)	92		70 - 121
4-Bromofluorobenzene (Surr)	84		59 - 120
Toluene-d8 (Surr)	86		70 - 123
Dibromofluoromethane (Surr)	101		75 - 128

Lab Sample ID: MRL 240-369935/5

Matrix: Water

Analysis Batch: 369935

Client Sample ID: Lab Control Sample

Prep Type: Total/NA

Analyte	Spike Added	MRL Result	MRL Qualifier	Unit	D	%Rec	%Rec. Limits
Vinyl chloride	0.00100	0.000822	J	ng/uL		82	10 - 150

Lab Sample ID: 240-108594-E-3 MS

Matrix: Water

Analysis Batch: 369935

Client Sample ID: Matrix Spike

Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	%Rec. Limits
1,1-Dichloroethene	22		10.0	28.1		ug/L		64	53 - 140
cis-1,2-Dichloroethene	3.9		10.0	15.3		ug/L		114	64 - 130
Tetrachloroethene	1.0	U	10.0	9.76		ug/L		98	51 - 136
trans-1,2-Dichloroethene	1.0	U	10.0	12.0		ug/L		120	68 - 133
Trichloroethene	4.3		10.0	14.9		ug/L		107	55 - 131

TestAmerica Canton

QC Sample Results

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Method: 8260B - Volatile Organic Compounds (GC/MS) (Continued)

Lab Sample ID: 240-108594-E-3 MS

Matrix: Water

Analysis Batch: 369935

Client Sample ID: Matrix Spike

Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	%Rec. Limits
Vinyl chloride	1.0	U	10.0	8.75		ug/L		87	43 - 154
Surrogate	MS %Recovery	MS Qualifier	Limits						
1,2-Dichloroethane-d4 (Surr)	91		70 - 121						
4-Bromofluorobenzene (Surr)	80		59 - 120						
Toluene-d8 (Surr)	81		70 - 123						
Dibromofluoromethane (Surr)	101		75 - 128						

Lab Sample ID: 240-108594-H-3 MSD

Matrix: Water

Analysis Batch: 369935

Client Sample ID: Matrix Spike Duplicate

Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MSD Result	MSD Qualifier	Unit	D	%Rec	%Rec. Limits	RPD	RPD Limit
1,1-Dichloroethene	22		10.0	29.3		ug/L		76	53 - 140	4	35
cis-1,2-Dichloroethene	3.9		10.0	15.1		ug/L		112	64 - 130	2	21
Tetrachloroethene	1.0	U	10.0	9.93		ug/L		99	51 - 136	2	23
trans-1,2-Dichloroethene	1.0	U	10.0	11.9		ug/L		119	68 - 133	1	24
Trichloroethene	4.3		10.0	14.8		ug/L		105	55 - 131	1	23
Vinyl chloride	1.0	U	10.0	10.6		ug/L		106	43 - 154	20	29
Surrogate	MSD %Recovery	MSD Qualifier	Limits								
1,2-Dichloroethane-d4 (Surr)	89		70 - 121								
4-Bromofluorobenzene (Surr)	81		59 - 120								
Toluene-d8 (Surr)	81		70 - 123								
Dibromofluoromethane (Surr)	99		75 - 128								

Method: 8260B SIM - Volatile Organic Compounds (GC/MS)

Lab Sample ID: MB 240-370005/5

Matrix: Water

Analysis Batch: 370005

Client Sample ID: Method Blank

Prep Type: Total/NA

Analyte	MB Result	MB Qualifier	RL	MDL	Unit	D	Prepared	Analyzed	Dil Fac
1,4-Dioxane	2.0	U	2.0	0.86	ug/L			03/02/19 13:07	1
Surrogate	MB %Recovery	MB Qualifier	Limits				Prepared	Analyzed	Dil Fac
1,2-Dichloroethane-d4 (Surr)	80		63 - 125					03/02/19 13:07	1

Lab Sample ID: LCS 240-370005/4

Matrix: Water

Analysis Batch: 370005

Client Sample ID: Lab Control Sample

Prep Type: Total/NA

Analyte	Spike Added	LCS Result	LCS Qualifier	Unit	D	%Rec	%Rec. Limits
1,4-Dioxane	10.0	11.8		ug/L		118	59 - 131
Surrogate	LCS %Recovery	LCS Qualifier	Limits				
1,2-Dichloroethane-d4 (Surr)	84		63 - 125				

TestAmerica Canton

QC Sample Results

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Lab Sample ID: 240-108589-B-1 MS
Matrix: Water
Analysis Batch: 370005

Client Sample ID: Matrix Spike
Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	%Rec. Limits
1,4-Dioxane	11		10.0	22.7		ug/L		119	52 - 129
Surrogate	%Recovery	MS Qualifier	MS Limits						
1,2-Dichloroethane-d4 (Surr)	82		63 - 125						

Lab Sample ID: 240-108589-B-1 MSD
Matrix: Water
Analysis Batch: 370005

Client Sample ID: Matrix Spike Duplicate
Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MSD Result	MSD Qualifier	Unit	D	%Rec	%Rec. Limits	RPD	RPD Limit
1,4-Dioxane	11		10.0	21.2		ug/L		104	52 - 129	7	13
Surrogate	%Recovery	MSD Qualifier	MSD Limits								
1,2-Dichloroethane-d4 (Surr)	82		63 - 125								

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

QC Association Summary

Client: ARCADIS U.S., Inc.
 Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

GC/MS VOA

Analysis Batch: 369935

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
240-108701-1	MW-131S_022619	Total/NA	Water	8260B	
240-108701-2	MW-132S_022619	Total/NA	Water	8260B	
240-108701-3	MW-85_022619	Total/NA	Water	8260B	
240-108701-4	MW-78S_022619	Total/NA	Water	8260B	
240-108701-5	MW-78_022619	Total/NA	Water	8260B	
240-108701-6	TRIP BLANK	Total/NA	Water	8260B	
MB 240-369935/6	Method Blank	Total/NA	Water	8260B	
LCS 240-369935/4	Lab Control Sample	Total/NA	Water	8260B	
MRL 240-369935/5	Lab Control Sample	Total/NA	Water	8260B	
240-108594-E-3 MS	Matrix Spike	Total/NA	Water	8260B	
240-108594-H-3 MSD	Matrix Spike Duplicate	Total/NA	Water	8260B	

Analysis Batch: 370005

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
240-108701-1	MW-131S_022619	Total/NA	Water	8260B SIM	
240-108701-2	MW-132S_022619	Total/NA	Water	8260B SIM	
240-108701-3	MW-85_022619	Total/NA	Water	8260B SIM	
240-108701-4	MW-78S_022619	Total/NA	Water	8260B SIM	
240-108701-5	MW-78_022619	Total/NA	Water	8260B SIM	
MB 240-370005/5	Method Blank	Total/NA	Water	8260B SIM	
LCS 240-370005/4	Lab Control Sample	Total/NA	Water	8260B SIM	
240-108589-B-1 MS	Matrix Spike	Total/NA	Water	8260B SIM	
240-108589-B-1 MSD	Matrix Spike Duplicate	Total/NA	Water	8260B SIM	

Lab Chronicle

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Client Sample ID: MW-131S_022619

Date Collected: 02/26/19 09:47

Date Received: 02/28/19 08:00

Lab Sample ID: 240-108701-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Analysis	8260B		1	369935	03/01/19 19:47	LEE	TAL CAN
Total/NA	Analysis	8260B SIM		1	370005	03/02/19 18:58	SAM	TAL CAN

Client Sample ID: MW-132S_022619

Date Collected: 02/26/19 11:22

Date Received: 02/28/19 08:00

Lab Sample ID: 240-108701-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Analysis	8260B		1	369935	03/01/19 20:09	LEE	TAL CAN
Total/NA	Analysis	8260B SIM		1	370005	03/02/19 19:23	SAM	TAL CAN

Client Sample ID: MW-85_022619

Date Collected: 02/26/19 13:23

Date Received: 02/28/19 08:00

Lab Sample ID: 240-108701-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Analysis	8260B		1	369935	03/01/19 20:31	LEE	TAL CAN
Total/NA	Analysis	8260B SIM		1	370005	03/02/19 19:48	SAM	TAL CAN

Client Sample ID: MW-78S_022619

Date Collected: 02/26/19 15:47

Date Received: 02/28/19 08:00

Lab Sample ID: 240-108701-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Analysis	8260B		1	369935	03/01/19 20:53	LEE	TAL CAN
Total/NA	Analysis	8260B SIM		1	370005	03/02/19 20:13	SAM	TAL CAN

Client Sample ID: MW-78_022619

Date Collected: 02/26/19 16:40

Date Received: 02/28/19 08:00

Lab Sample ID: 240-108701-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Analysis	8260B		1	369935	03/01/19 21:15	LEE	TAL CAN
Total/NA	Analysis	8260B SIM		1	370005	03/02/19 20:38	SAM	TAL CAN

Client Sample ID: TRIP BLANK

Date Collected: 02/26/19 00:00

Date Received: 02/28/19 08:00

Lab Sample ID: 240-108701-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Analysis	8260B		1	369935	03/01/19 21:37	LEE	TAL CAN

TestAmerica Canton

Lab Chronicle

Client: ARCADIS U.S., Inc.
Project/Site: Ford LTP Livonia MI - E203631

TestAmerica Job ID: 240-108701-1

Laboratory References:

TAL CAN = TestAmerica Canton, 4101 Shuffel Street NW, North Canton, OH 44720, TEL (330)497-9396

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14

Accreditation/Certification Summary

Client: ARCADIS U.S., Inc.

TestAmerica Job ID: 240-108701-1

Project/Site: Ford LTP Livonia MI - E203631

Laboratory: TestAmerica Canton

All accreditations/certifications held by this laboratory are listed. Not all accreditations/certifications are applicable to this report.

Authority	Program	EPA Region	Identification Number	Expiration Date
California	State Program	9	2927	02-23-20
Connecticut	State Program	1	PH-0590	12-31-19
Florida	NELAP	4	E87225	06-30-19
Illinois	NELAP	5	200004	07-31-19
Kansas	NELAP	7	E-10336	04-30-19 *
Kentucky (UST)	State Program	4	58	02-23-20
Kentucky (WW)	State Program	4	98016	12-31-19
Minnesota	NELAP	5	039-999-348	12-31-19 *
Minnesota (Petrofund)	State Program	1	3506	07-31-19
Nevada	State Program	9	OH00048	07-31-19
New Jersey	NELAP	2	OH001	06-30-19
New York	NELAP	2	10975	03-31-19 *
Ohio VAP	State Program	5	CL0024	09-06-19
Oregon	NELAP	10	4062	02-23-20
Pennsylvania	NELAP	3	68-00340	08-31-19 *
Texas	NELAP	6	T104704517-18-10	08-31-19
USDA	Federal		P330-16-00404	12-28-19
Virginia	NELAP	3	460175	09-14-19
Washington	State Program	10	C971	01-12-20 *
West Virginia DEP	State Program	3	210	12-31-19

* Accreditation/Certification renewal pending - accreditation/certification considered valid.

TestAmerica Canton


TestAmerica Canton Sample Receipt Form/Narrative
Canton Facility

Login #: 108701

Client Accalis Site Name _____ Cooler unpacked by: SC
Cooler Received on 2/28/19 Opened on 2/28/19
FedEx: 1st Grd Exp UPS FAS Clipper Client Drop Off/ TestAmerica Courier Other _____

Receipt After-hours: Drop-off Date/Time _____ Storage Location _____

TestAmerica Cooler # TA Foam Box Client Cooler Box Other _____
Packing material used: Bubble Wrap Foam Plastic Bag None Other _____
COOLANT: Wet Ice Blue Ice Dry Ice Water None

1. Cooler temperature upon receipt See Multiple Cooler Form
IR GUN# IR-8 (CF -0.2 °C) Observed Cooler Temp. 2.8 °C Corrected Cooler Temp. 2.6 °C
IR GUN #36 (CF +0.7°C) Observed Cooler Temp. _____ °C Corrected Cooler Temp. _____ °C
2. Were tamper/custody seals on the outside of the cooler(s)? If Yes Quantity 1 Yes No
-Were the seals on the outside of the cooler(s) signed & dated? Yes No NA
-Were tamper/custody seals on the bottle(s) or bottle kits (LLHg/MeHg)? Yes No NA
-Were tamper/custody seals intact and uncompromised? Yes No NA
3. Shippers' packing slip attached to the cooler(s)? Yes No
4. Did custody papers accompany the sample(s)? Yes No
5. Were the custody papers relinquished & signed in the appropriate place? Yes No
6. Was/were the person(s) who collected the samples clearly identified on the COC? Yes No
7. Did all bottles arrive in good condition (Unbroken)? Yes No
8. Could all bottle labels be reconciled with the COC? Yes No
9. Were correct bottle(s) used for the test(s) indicated? Yes No
10. Sufficient quantity received to perform indicated analyses? Yes No
11. Are these work share samples? Yes No
If yes, Questions 12-16 have been checked at the originating laboratory.
12. Were all preserved sample(s) at the correct pH upon receipt? Yes No NA pH Strip Lot# HC861525
13. Were VOAs on the COC? Yes No
14. Were air bubbles >6 mm in any VOA vials? Yes No NA
 Larger than this.
15. Was a VOA trip blank present in the cooler(s)? Trip Blank Lot # 831707 Yes No
16. Was a LL Hg or Me Hg trip blank present? Yes No

Tests that are not checked for pH by Receiving:
VOAs
Oil and Grease
TOC

Contacted PM _____ Date _____ by _____ via Verbal Voice Mail Other _____
Concerning _____

17. CHAIN OF CUSTODY & SAMPLE DISCREPANCIES

Samples processed by: RC

18. SAMPLE CONDITION

Sample(s) _____ were received after the recommended holding time had expired.
Sample(s) _____ were received in a broken container.
Sample(s) _____ were received with bubble >6 mm in diameter. (Notify PM)

19. SAMPLE PRESERVATION

Sample(s) _____ were further preserved in the laboratory.
Time preserved: _____ Preservative(s) added/Lot number(s): _____
VOA Sample Preservation - Date/Time VOAs Frozen: _____